

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
 Data File : VU061157.D
 Acq On : 18 Oct 2024 11:34
 Operator : MD/SY
 Sample : VU1018WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1018WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU061157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.033	534	542	543	rBV2	2134	1615	2.10%	0.566%
2	3.181	576	588	596	rBV2	1623	2997	3.90%	1.051%
3	3.689	737	746	748	rBV3	2931	3579	4.66%	1.255%
4	4.634	1029	1040	1041	rBV	1401	1441	1.88%	0.505%
5	6.110	1485	1499	1524	rBV	26242	56294	73.25%	19.736%
6	7.981	2078	2081	2090	rVB4	818	950	1.24%	0.333%
7	8.463	2224	2231	2238	rBV3	988	1370	1.78%	0.480%
8	9.573	2568	2576	2584	rBV3	1006	1658	2.16%	0.581%
9	9.701	2603	2616	2630	rBV3	2107	4304	5.60%	1.509%
10	10.097	2728	2739	2741	rBV3	1093	1203	1.57%	0.422%
11	10.483	2852	2859	2866	rBB3	1091	1522	1.98%	0.534%
12	10.634	2896	2906	2929	rBV2	30283	57302	74.56%	20.090%
13	10.782	2947	2952	2961	rVB3	763	997	1.30%	0.350%
14	10.881	2975	2983	2984	rBV3	1234	1166	1.52%	0.409%
15	10.907	2988	2991	2996	rVV	1406	1539	2.00%	0.540%
16	11.087	3040	3047	3051	rBV2	1230	1434	1.87%	0.503%
17	11.415	3143	3149	3154	rBV2	870	1189	1.55%	0.417%
18	11.476	3158	3168	3179	rVB4	1191	1962	2.55%	0.688%
19	11.637	3212	3218	3230	rVB3	1159	1994	2.59%	0.699%
20	11.759	3250	3256	3261	rBV5	1206	1441	1.88%	0.505%
21	11.846	3278	3283	3291	rVB5	962	1309	1.70%	0.459%
22	12.190	3380	3390	3412	rBV	40846	76849	100.00%	26.943%
23	12.762	3558	3568	3579	rBV	4503	6785	8.83%	2.379%
24	13.862	3902	3910	3919	rVB4	1520	2551	3.32%	0.894%
25	14.116	3980	3989	3991	rBV3	1314	1665	2.17%	0.584%
26	14.338	4051	4058	4071	rVB6	2186	3546	4.61%	1.243%
27	14.569	4114	4130	4141	rVB	24385	38739	50.41%	13.582%
28	15.875	4530	4536	4542	rVB5	643	776	1.01%	0.272%
29	16.177	4619	4630	4640	rBV2	3746	6250	8.13%	2.191%
30	17.196	4944	4947	4949	rBV3	1160	801	1.04%	0.281%




Sum of corrected areas: 285228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
Data File : VU061157.D
Acq On : 18 Oct 2024 11:34
Operator : MD/SY
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

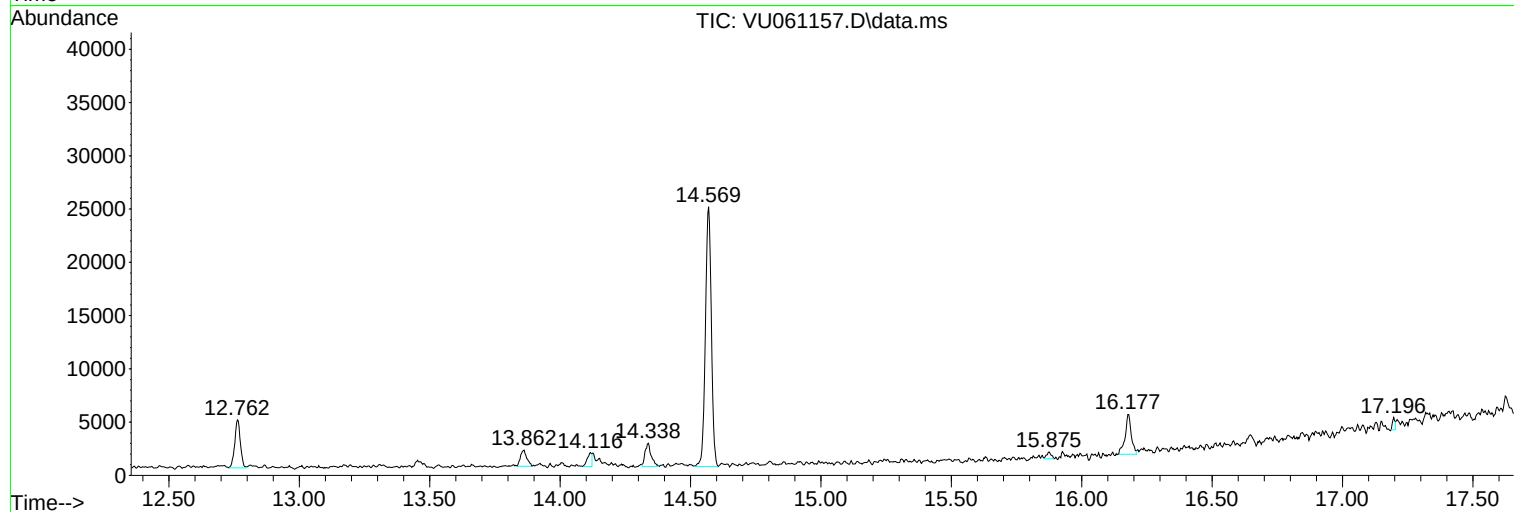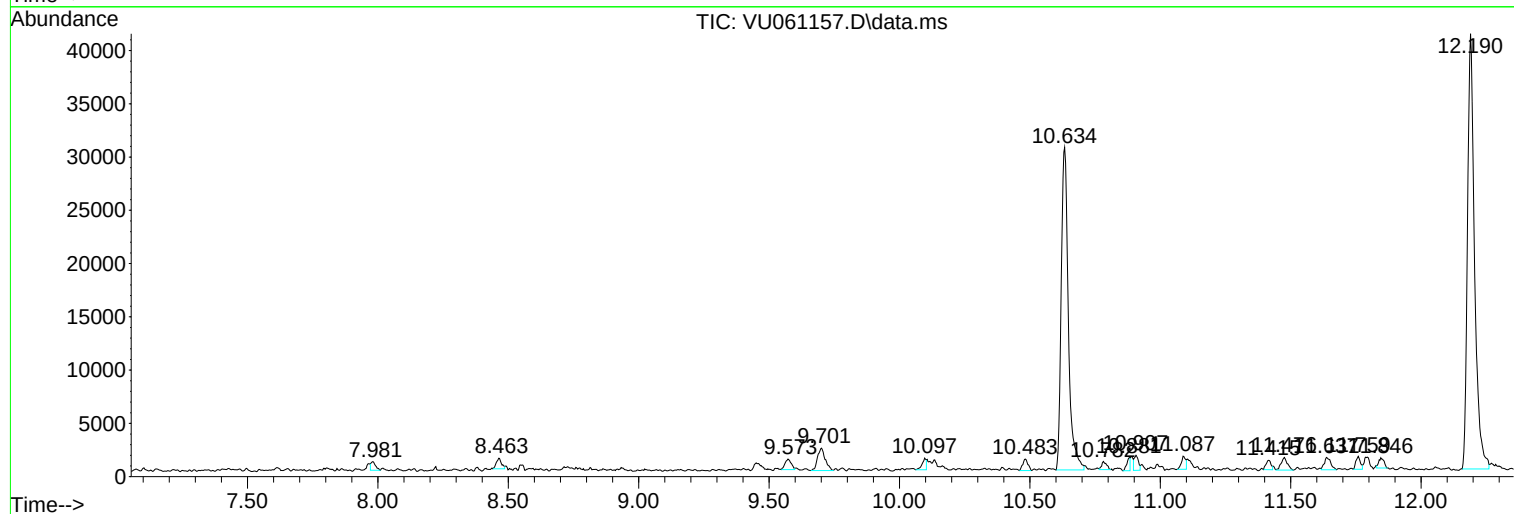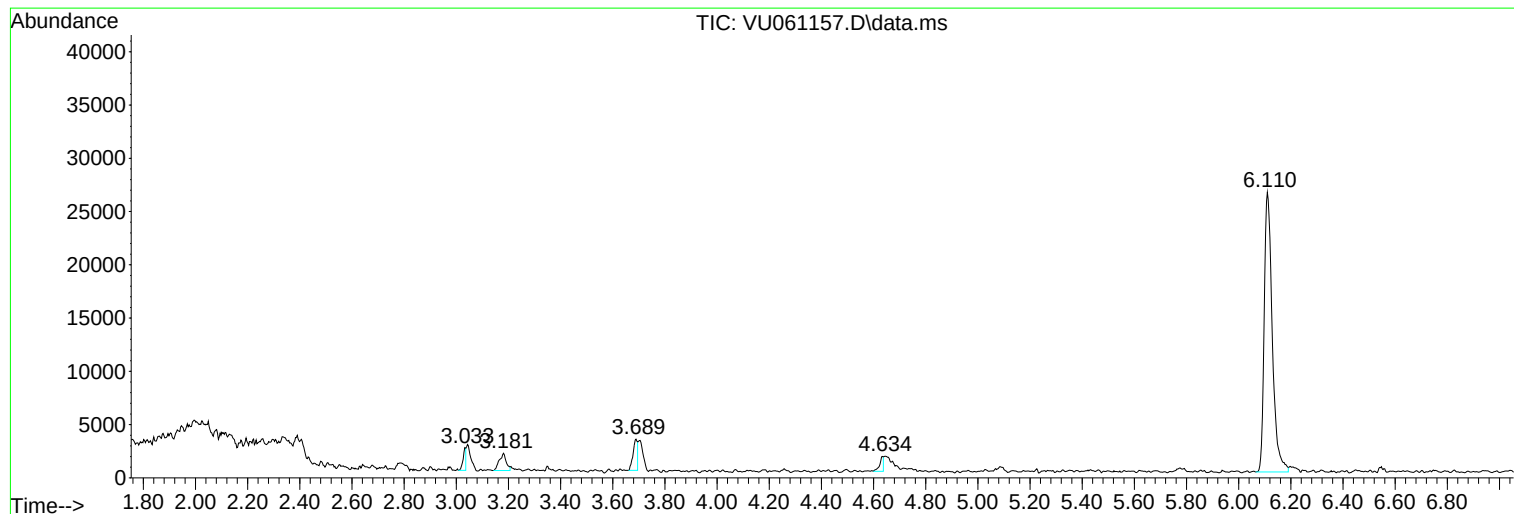

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
Data File : VU061157.D
Acq On : 18 Oct 2024 11:34
Operator : MD/SY
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
Data File : VU061157.D
Acq On : 18 Oct 2024 11:34
Operator : MD/SY
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------