

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
 Data File : VU061168.D
 Acq On : 21 Oct 2024 13:15
 Operator : MD/SY
 Sample : VU1021WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1021WBL01

Quant Time: Oct 22 01:21:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Oct 18 02:52:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	28097	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	13383	0.896	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12519	0.851	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
Data File : VU061168.D
Acq On : 21 Oct 2024 13:15
Operator : MD/SY
Sample : VU1021WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01

Quant Time: Oct 22 01:21:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Oct 18 02:52:28 2024
Response via : Initial Calibration




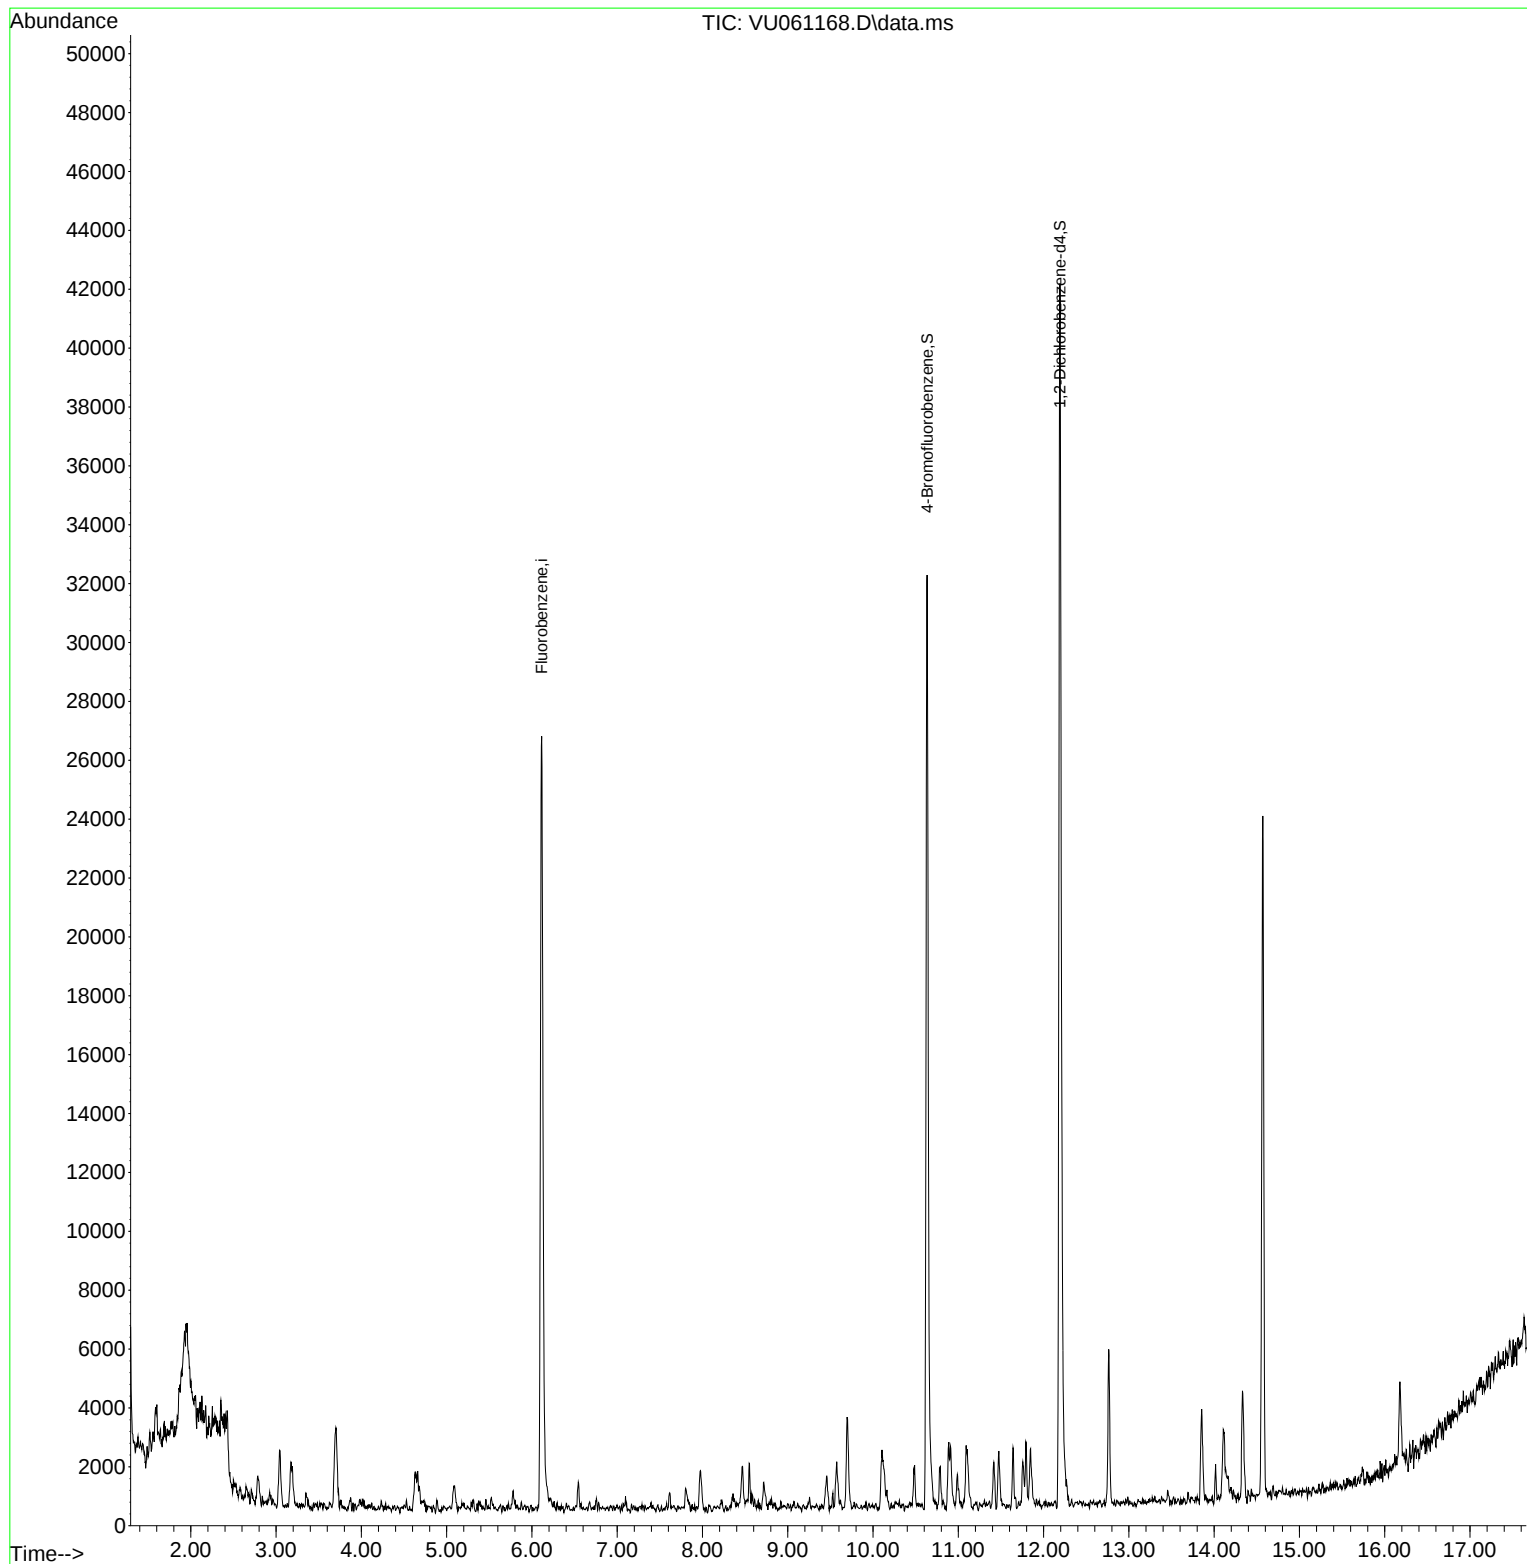


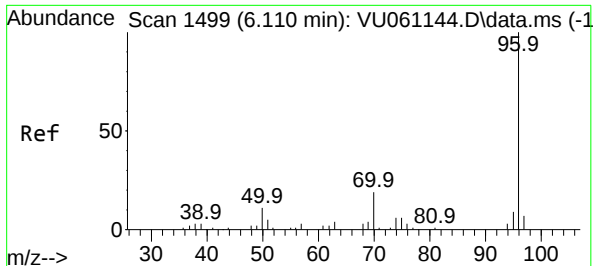

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU061168.D
Acq: 21 Oct 2024 13:15




Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01


Tgt Ion:	96	Resp:	28097
Ion Ratio	Lower	Upper	
96	100		
70	18.0	16.1	24.1
95	7.6	0.0	0.0#
97	5.9	0.0	0.0#

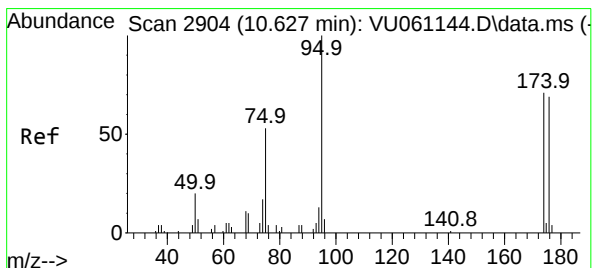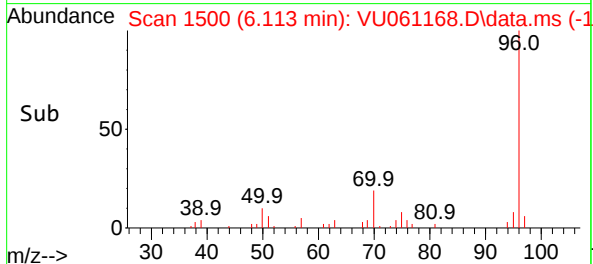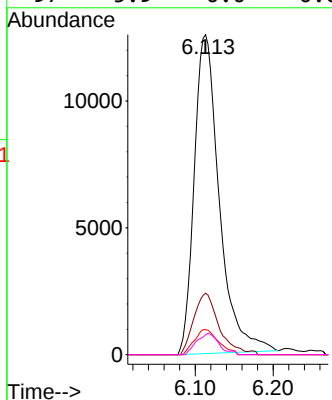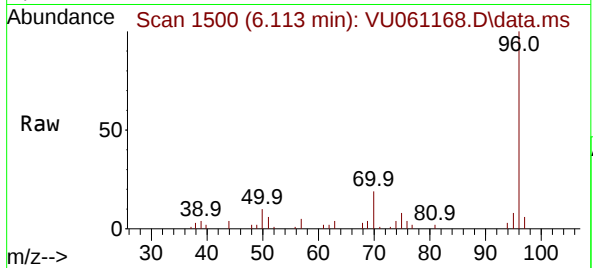

#57
4-Bromofluorobenzene
Concen: 0.896 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.006 min
Lab File: VU061168.D
Acq: 21 Oct 2024 13:15

Tgt Ion:	95	Resp:	13383
Ion Ratio	Lower	Upper	
95	100		
174	72.6	55.4	83.0
176	72.0	54.4	81.6

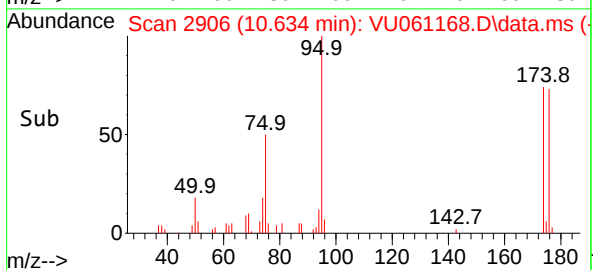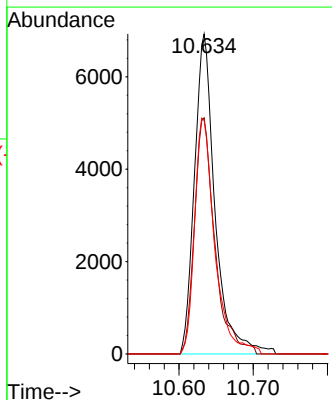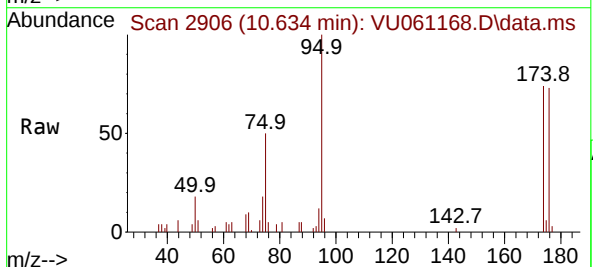

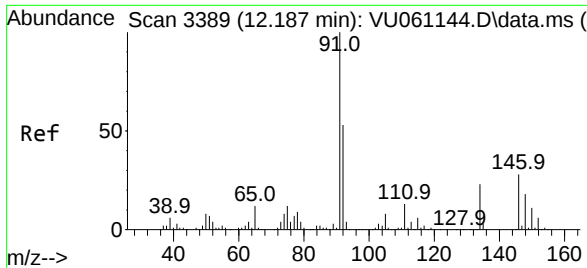

#68

1,2-Dichlorobenzene-d4

Concen: 0.851 ug/l

RT: 12.190 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU061168.D


Acq: 21 Oct 2024 13:15

Instrument :

MSVOA_U

ClientSampleId :

VU1021WBL01

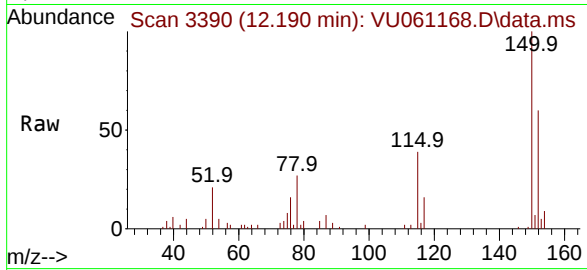

Tgt Ion:152 Resp: 12519

Ion Ratio Lower Upper

152 100

115 66.0 0.0 275.0

150 160.1 0.0 668.8

