

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
 Data File : VU061168.D
 Acq On : 21 Oct 2024 13:15
 Operator : MD/SY
 Sample : VU1021WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1021WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU061168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.859	174	177	180	rBV4	962	864	1.03%	0.251%
2	2.351	327	330	334	rBV4	1243	1205	1.44%	0.350%
3	2.785	455	465	478	rVB2	1011	2281	2.72%	0.662%
4	3.043	533	545	557	rBV3	1960	3743	4.46%	1.087%
5	3.174	576	586	589	rBV4	1539	2314	2.76%	0.672%
6	3.702	735	750	758	rBV7	2707	6285	7.49%	1.824%
7	4.631	1028	1039	1041	rBV3	1340	1921	2.29%	0.558%
8	4.660	1045	1048	1051	rVV2	1203	1083	1.29%	0.314%
9	5.087	1170	1181	1188	rBV3	782	1602	1.91%	0.465%
10	6.113	1489	1500	1525	rBV	26154	55048	65.63%	15.980%
11	6.544	1628	1634	1640	rVB3	852	1079	1.29%	0.313%
12	7.801	2020	2025	2033	rBV6	657	1067	1.27%	0.310%
13	7.975	2069	2079	2090	rVB3	1319	2627	3.13%	0.763%
14	8.467	2222	2232	2239	rBV2	1228	1879	2.24%	0.545%
15	8.547	2253	2257	2264	rVB5	1359	1422	1.70%	0.413%
16	8.718	2301	2310	2320	rBV4	939	1834	2.19%	0.532%
17	9.457	2528	2540	2550	rVB3	1166	2415	2.88%	0.701%
18	9.573	2568	2576	2586	rBV3	1515	2619	3.12%	0.760%
19	9.695	2604	2614	2626	rBV2	3070	5553	6.62%	1.612%
20	10.103	2729	2741	2756	rBV7	2045	5488	6.54%	1.593%
21	10.486	2851	2860	2867	rVB4	1377	1917	2.29%	0.556%
22	10.634	2895	2906	2928	rBV2	31747	58773	70.07%	17.061%
23	10.788	2942	2954	2958	rBV4	1453	2187	2.61%	0.635%
24	10.888	2976	2985	2988	rBV3	2310	3270	3.90%	0.949%
25	10.907	2988	2991	3005	rVB3	1970	2735	3.26%	0.794%
26	10.988	3009	3016	3019	rBV4	996	1120	1.34%	0.325%
27	11.090	3041	3048	3051	rBV3	1897	2142	2.55%	0.622%
28	11.415	3138	3149	3158	rVB5	1601	2646	3.15%	0.768%
29	11.473	3158	3167	3176	rBV3	1978	3280	3.91%	0.952%
30	11.640	3210	3219	3226	rBV3	2095	2879	3.43%	0.836%
31	11.756	3245	3255	3261	rBV6	1488	2408	2.87%	0.699%
32	11.791	3261	3266	3276	rVV2	2146	2874	3.43%	0.834%
33	11.846	3276	3283	3297	rVB4	1870	3280	3.91%	0.952%
34	12.190	3379	3390	3413	rBV2	41600	83880	100.00%	24.349%
35	12.762	3555	3568	3580	rBV2	5313	8105	9.66%	2.353%
36	13.852	3899	3907	3918	rBV7	3234	5743	6.85%	1.667%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
Data File : VU061168.D
Acq On : 21 Oct 2024 13:15
Operator : MD/SY
Sample : VU1021WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

37	14.016	3951	3958	3963	rBV4	1361	1464	1.75%	0.425%
38	14.106	3977	3986	3993	rBV4	2275	4266	5.09%	1.238%
39	14.331	4046	4056	4069	rBV5	3665	6694	7.98%	1.943%
40	14.569	4118	4130	4141	rBV	22993	37574	44.79%	10.907%
41	16.177	4623	4630	4639	rVB4	2526	4006	4.78%	1.163%
42	16.293	4660	4666	4669	rBV4	943	919	1.10%	0.267%




Sum of corrected areas: 344491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
Data File : VU061168.D
Acq On : 21 Oct 2024 13:15
Operator : MD/SY
Sample : VU1021WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

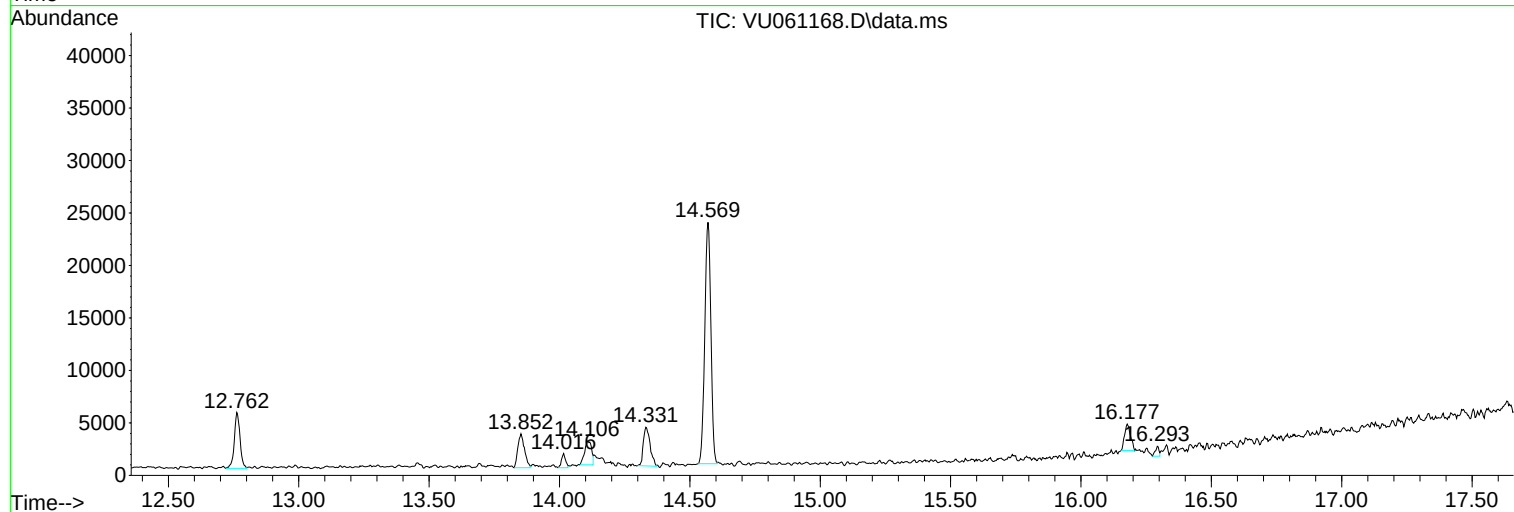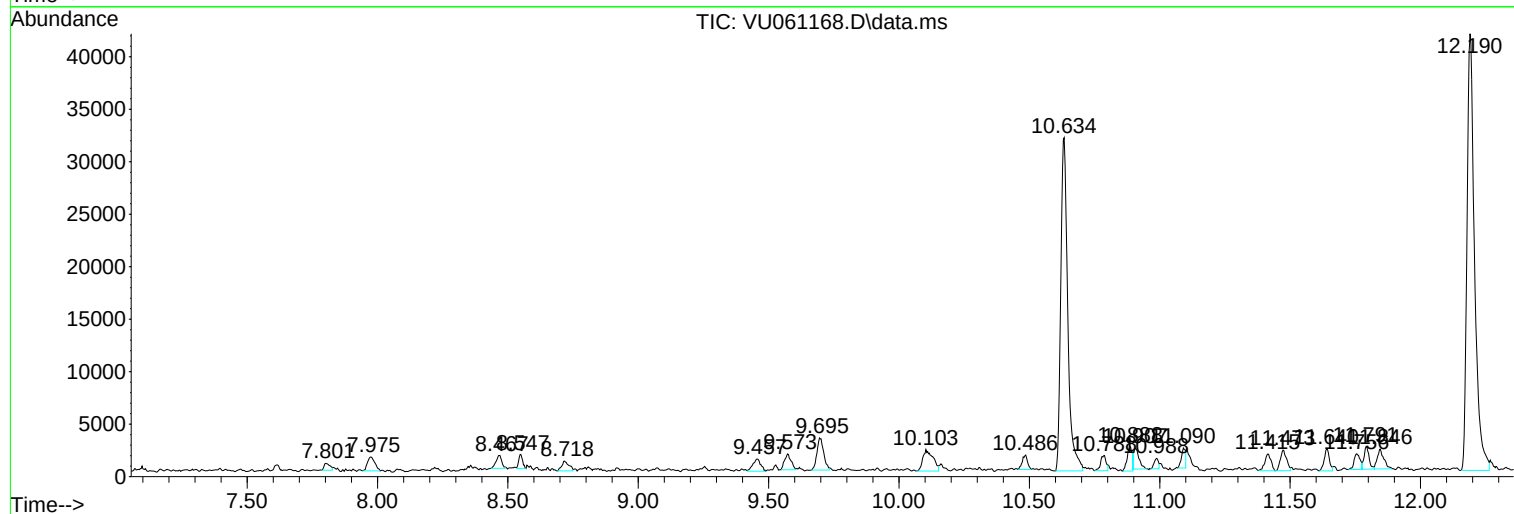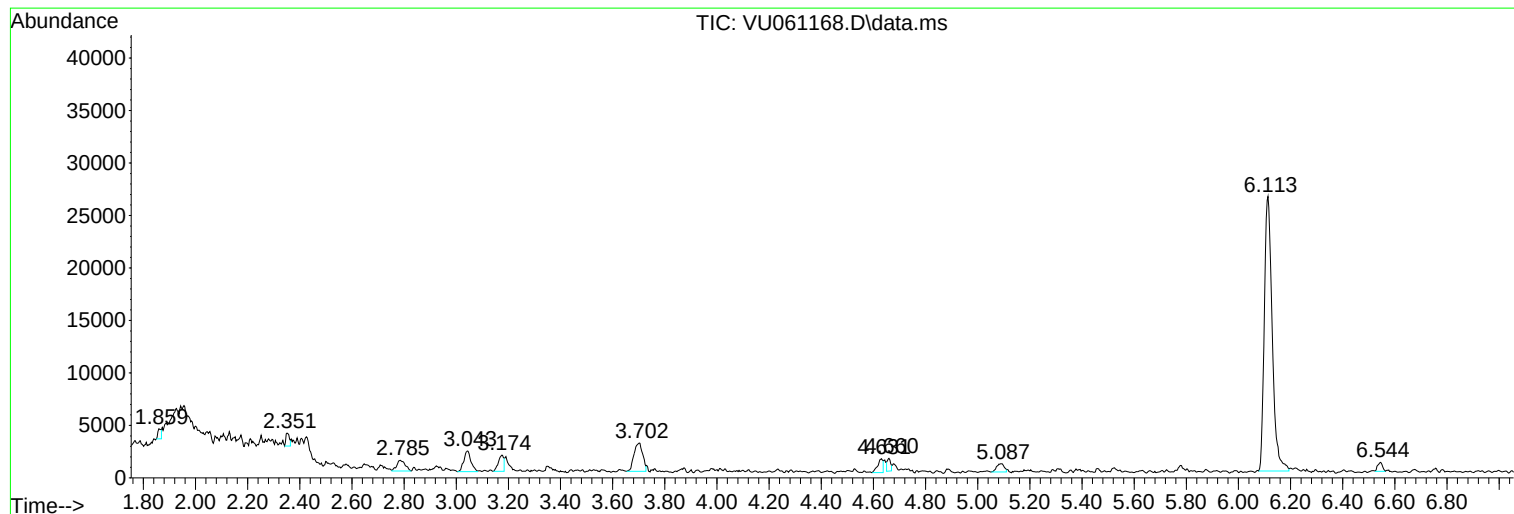

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
Data File : VU061168.D
Acq On : 21 Oct 2024 13:15
Operator : MD/SY
Sample : VU1021WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102124\
Data File : VU061168.D
Acq On : 21 Oct 2024 13:15
Operator : MD/SY
Sample : VU1021WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1021WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------