
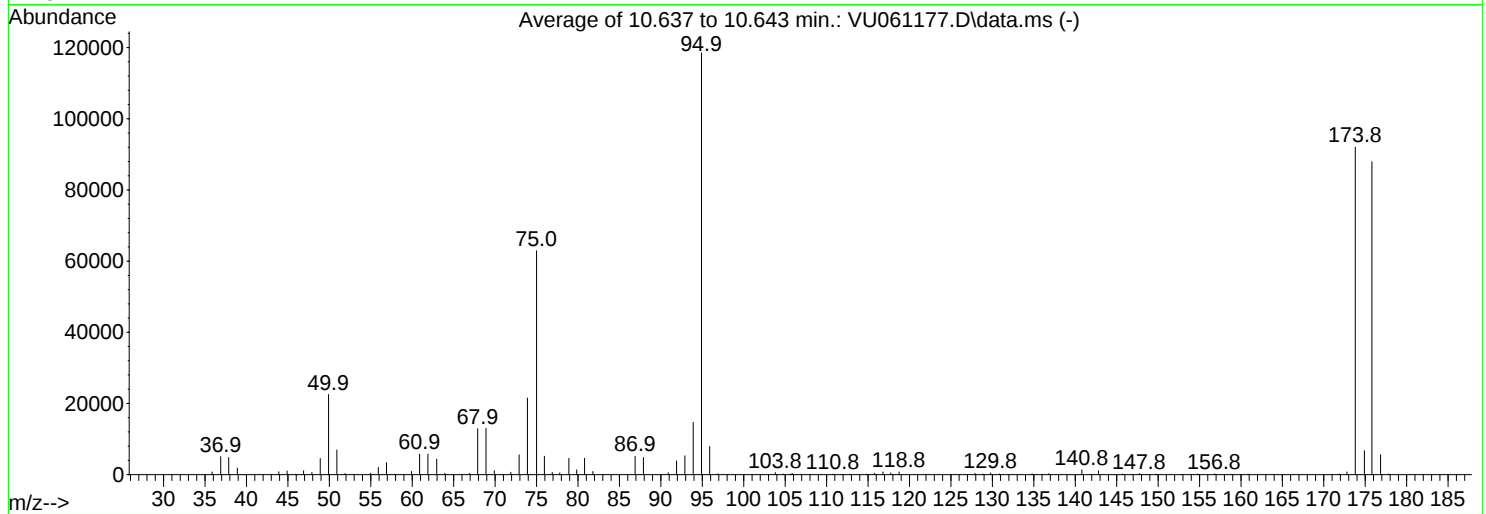


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102224\
Data File : VU061177.D
Acq On : 22 Oct 2024 08:43
Operator : MD/SY
Sample : BFB017
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB017

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM102224.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 23 02:31:01 2024

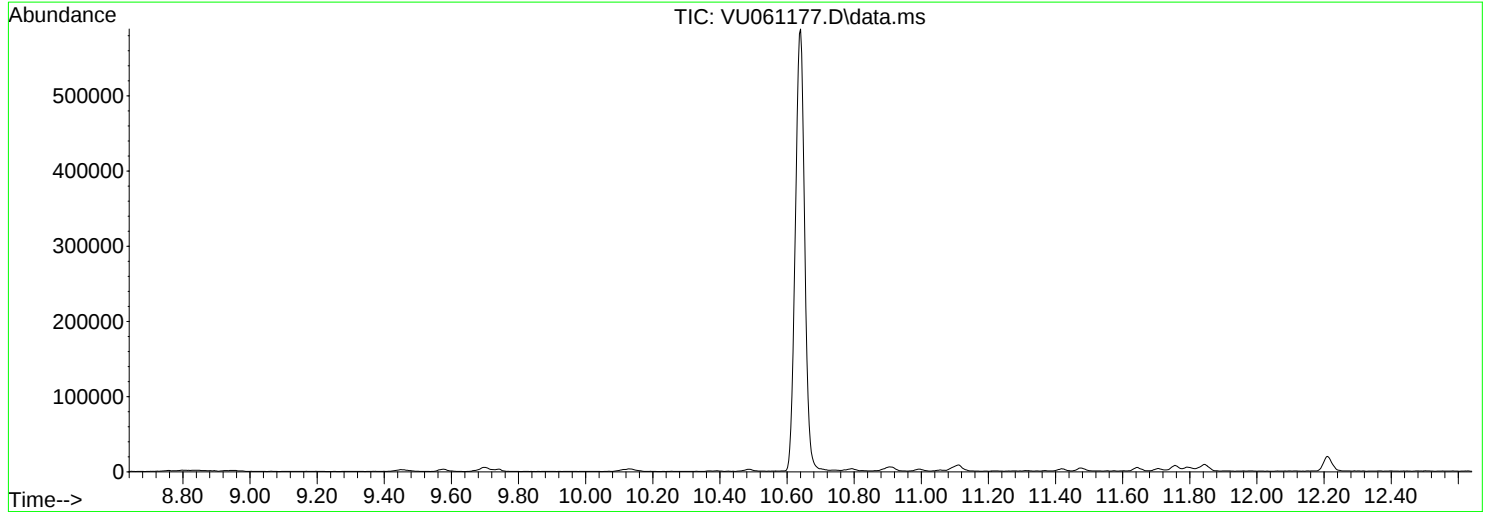

AutoFind: Scans 2907, 2908, 2909; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22523	PASS
75	95	30	80	53.1	62896	PASS
95	95	100	100	100.0	118533	PASS
96	95	5	9	6.7	7923	PASS
173	174	0.00	2	0.9	785	PASS
174	95	50	120	77.7	92051	PASS
175	174	5	9	7.3	6731	PASS
176	174	95	101	95.6	87965	PASS
177	176	5	9	6.4	5645	PASS

m/z	Abundance
35.80	378.0
37.80	105.0
39.80	268.0
42.90	139.0
43.90	380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	1144.0
36.90	5184.0
37.90	5039.0
38.90	1974.0
39.90	263.0
42.80	116.0
43.90	1223.0
44.90	1035.0
45.90	156.0
46.90	1140.0
47.90	619.0
48.90	4561.0
49.90	23128.0
50.90	7277.0
51.90	358.0
55.00	422.0
55.90	1997.0
56.90	3430.0
57.90	148.0
59.90	951.0
60.90	5894.0
61.90	5874.0
63.00	4565.0
63.90	453.0
66.90	372.0
67.90	13274.0
68.90	13135.0
69.90	1090.0
71.90	723.0
72.90	5675.0
73.90	22168.0
75.00	63840.0
75.90	5207.0
76.90	682.0
77.80	469.0
78.90	4705.0
79.80	1283.0
80.80	4589.0
81.80	894.0
86.90	5429.0
87.90	4964.0
90.90	498.0
91.90	4017.0
92.90	5212.0
93.90	14791.0
94.90	120504.0
95.90	8198.0
96.90	254.0
103.80	529.0
104.70	159.0
105.70	522.0
106.90	133.0
110.70	131.0
111.80	114.0
112.80	123.0
114.80	158.0
115.80	438.0
116.80	763.0
117.80	501.0
118.70	760.0
127.90	385.0
128.80	159.0
129.80	436.0
130.90	129.0
134.80	214.0
136.80	268.0
140.80	1409.0
142.80	1013.0
145.70	198.0
147.80	326.0
148.70	105.0
149.70	170.0
152.80	102.0
154.80	222.0
156.80	289.0
158.80	157.0
160.90	151.0
171.10	102.0
171.90	220.0
172.80	801.0
173.80	91480.0
174.90	6840.0
175.80	88208.0
176.80	5708.0
177.80	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	1143.0
36.90	5271.0
37.90	5026.0
38.90	1860.0
39.90	294.0
42.80	116.0
43.90	1203.0
44.90	1103.0
46.00	165.0
46.90	1141.0
47.90	632.0
48.90	4639.0
49.90	23144.0
50.90	7101.0
51.90	351.0
55.00	426.0
55.90	2093.0
56.90	3445.0
57.90	157.0
59.90	930.0
60.90	5899.0
61.90	5936.0
62.90	4383.0
63.90	407.0
66.90	365.0
67.90	13222.0
68.90	13400.0
69.90	1171.0
70.90	116.0
71.90	683.0
72.90	5674.0
73.90	21952.0
75.00	64392.0
75.90	5287.0
76.90	672.0
77.80	511.0
78.90	4768.0
79.80	1396.0
80.80	4708.0
81.80	945.0
85.80	105.0
86.90	5261.0
87.90	4847.0
90.90	543.0
91.90	3996.0
92.90	5419.0
93.90	15034.0
94.90	121056.0
95.90	8012.0
96.90	257.0
103.80	615.0
104.70	185.0
105.90	539.0
106.90	145.0
110.80	120.0
112.80	115.0
114.80	166.0
115.80	424.0
116.80	765.0
117.80	501.0
118.80	777.0
127.90	382.0
128.80	170.0
129.80	476.0
130.80	170.0
134.80	232.0
136.80	276.0
140.80	1387.0
141.70	109.0
142.80	1090.0
144.70	104.0
145.70	174.0
146.90	115.0
147.70	311.0
149.70	182.0
154.80	239.0
156.80	252.0
158.80	152.0
160.90	156.0
171.90	212.0
172.80	800.0
173.80	94104.0
174.90	6868.0
175.80	89984.0
176.80	5716.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	1155.0
36.90	4782.0
37.90	4700.0
38.90	1755.0
39.90	333.0
42.90	141.0
43.90	1189.0
44.90	1034.0
46.00	150.0
46.90	993.0
47.90	604.0
48.90	4431.0
49.90	21296.0
50.90	6431.0
51.90	333.0
54.90	325.0
55.90	1985.0
56.90	3243.0
57.90	150.0
59.90	851.0
60.90	5544.0
61.90	5534.0
62.90	4099.0
64.00	365.0
66.90	320.0
67.90	12207.0
68.90	12603.0
69.90	1111.0
70.90	131.0
71.90	638.0
72.90	5441.0
73.90	20552.0
75.00	60456.0
76.00	5053.0
76.90	607.0
77.80	513.0
78.90	4349.0
79.90	1321.0
80.80	4442.0
81.80	929.0
83.10	100.0
85.80	103.0
86.90	4877.0
87.90	4570.0
90.90	528.0
91.90	3644.0
92.90	5291.0
93.90	14302.0
94.90	114040.0
95.90	7559.0
96.90	278.0
103.80	629.0
104.80	209.0
105.80	551.0
106.90	120.0
110.80	112.0
112.80	109.0
114.80	142.0
115.80	395.0
116.80	707.0
117.70	481.0
118.80	734.0
127.90	376.0
128.90	181.0
129.80	472.0
130.80	210.0
134.80	236.0
136.80	272.0
140.80	1321.0
141.80	111.0
142.80	1083.0
144.80	103.0
145.80	146.0
146.90	127.0
147.70	270.0
149.80	175.0
154.80	240.0
156.80	186.0
158.80	131.0
160.80	140.0
171.80	178.0
172.80	753.0
173.80	90568.0
174.90	6484.0
175.80	85704.0
176.90	5510.0
177.90	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017