


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102324\
Data File : VU061187.D
Acq On : 23 Oct 2024 09:04
Operator : MD/SY
Sample : BFB013
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB013

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 24 01:26:37 2024

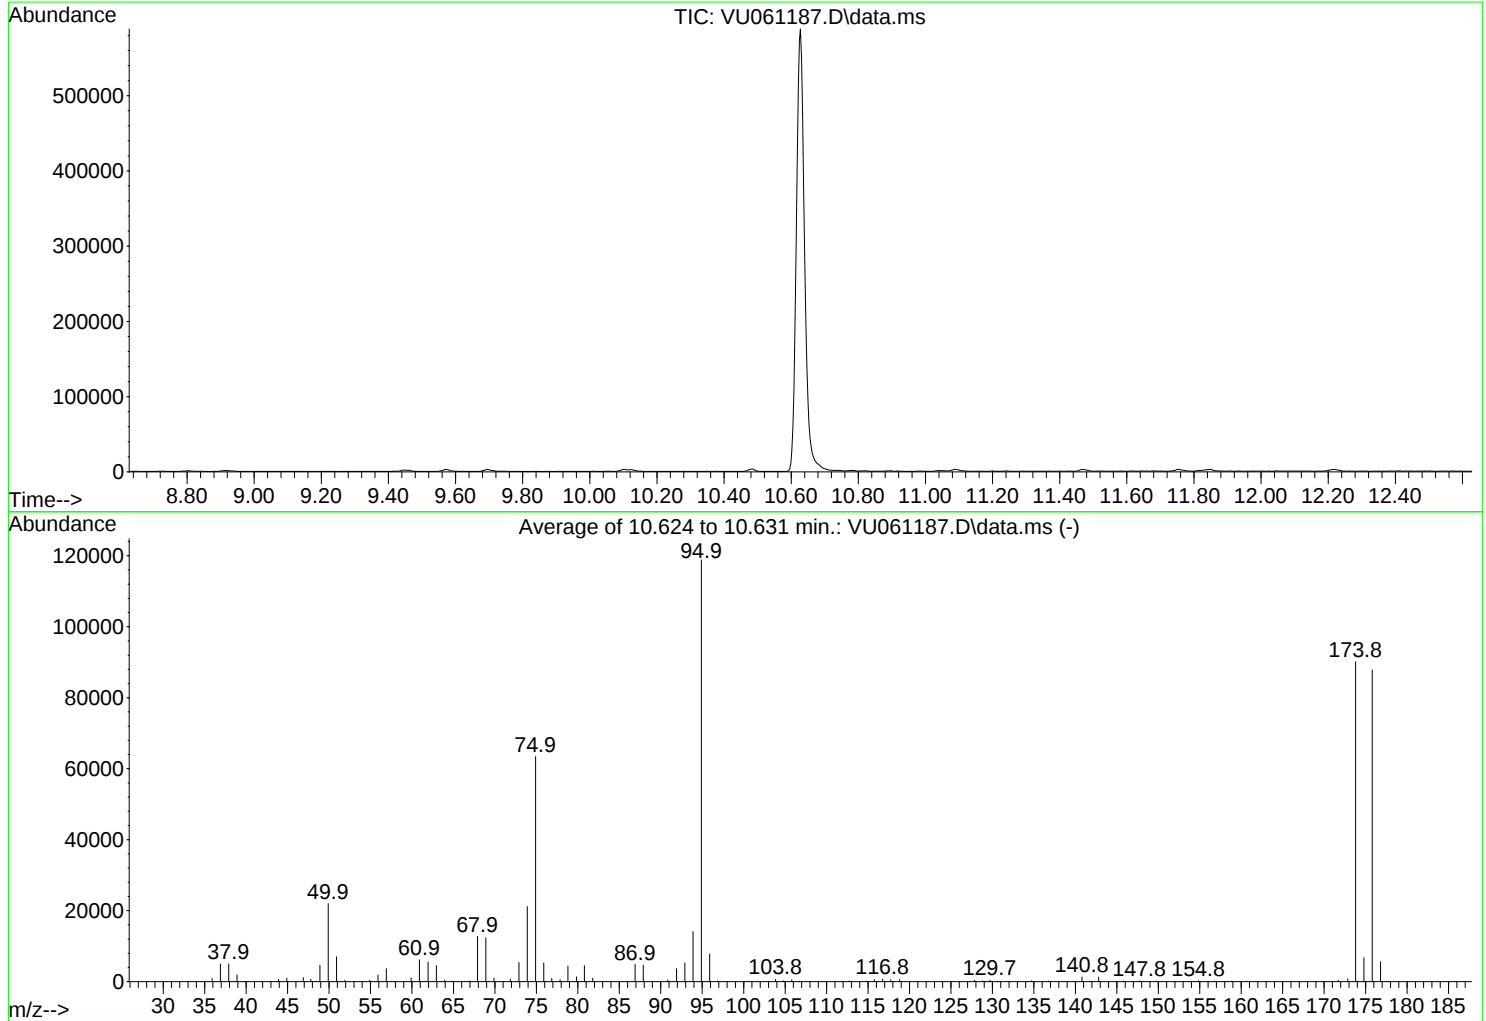

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	22016	PASS
75	95	30	80	53.3	63400	PASS
95	95	100	100	100.0	118859	PASS
96	95	5	9	6.6	7792	PASS
173	174	0.00	2	0.9	795	PASS
174	95	50	120	75.8	90131	PASS
175	174	5	9	7.5	6715	PASS
176	174	95	101	97.5	87851	PASS
177	176	5	9	6.4	5614	PASS

m/z	Abundance
39.70	231.0
43.90	413.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	864.0
36.90	5067.0
37.90	5143.0
38.90	2046.0
39.80	314.0
42.90	112.0
43.90	1025.0
44.90	1016.0
46.90	1211.0
47.80	676.0
48.90	4457.0
49.90	22384.0
50.90	7266.0
51.90	437.0
54.90	359.0
55.90	1890.0
56.90	3669.0
57.90	121.0
59.90	986.0
60.90	6278.0
62.00	5910.0
62.90	4646.0
63.90	388.0
64.80	123.0
66.80	307.0
67.90	12591.0
68.90	12668.0
69.90	982.0
71.90	681.0
72.90	5495.0
73.90	21576.0
74.90	64016.0
75.90	5506.0
76.80	928.0
77.90	530.0
78.80	4414.0
79.90	1400.0
80.80	4499.0
81.80	1004.0
83.00	109.0
85.90	151.0
86.90	4941.0
87.90	4740.0
90.90	507.0
91.90	3693.0
92.90	5369.0
93.90	14504.0
94.90	119952.0
95.90	8138.0
96.80	206.0
103.80	705.0
104.80	229.0
105.80	502.0
106.80	140.0
112.70	164.0
114.90	104.0
115.70	508.0
116.70	788.0
117.70	544.0
118.80	617.0
127.80	413.0
128.80	191.0
129.70	420.0
130.70	160.0
134.70	222.0
136.80	192.0
140.80	1430.0
141.70	121.0
142.80	1242.0
145.80	156.0
147.70	211.0
149.90	121.0
154.90	289.0
156.80	158.0
158.80	149.0
171.70	307.0
172.90	786.0
173.80	89072.0
174.80	6723.0
175.80	86496.0
176.80	5617.0
177.80	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	905.0
36.90	5152.0
37.90	5139.0
38.90	1947.0
39.80	305.0
43.90	1071.0
44.90	996.0
46.90	1205.0
47.80	708.0
48.90	4699.0
49.90	22736.0
50.90	7186.0
51.90	396.0
54.90	385.0
55.90	1917.0
56.90	3787.0
57.90	104.0
59.90	1056.0
60.90	6407.0
62.00	5684.0
62.90	4681.0
64.00	427.0
64.80	158.0
67.00	344.0
67.90	13207.0
68.90	12679.0
69.90	1025.0
71.90	641.0
72.90	5536.0
73.90	21664.0
74.90	65632.0
75.90	5446.0
76.90	925.0
77.90	550.0
78.80	4527.0
79.90	1413.0
80.80	4686.0
81.80	989.0
83.00	135.0
85.90	112.0
86.90	5026.0
87.90	4701.0
90.90	489.0
91.90	3735.0
92.90	5442.0
93.90	14387.0
94.90	122208.0
95.90	7975.0
96.90	197.0
103.80	700.0
104.80	235.0
105.80	566.0
106.70	124.0
111.80	101.0
112.70	182.0
114.80	126.0
115.80	556.0
116.80	746.0
117.70	568.0
118.80	599.0
127.90	390.0
128.80	219.0
129.70	408.0
130.70	124.0
134.70	237.0
136.80	177.0
139.80	114.0
140.80	1362.0
141.70	129.0
142.80	1312.0
144.90	104.0
145.80	193.0
147.80	222.0
149.80	126.0
154.80	290.0
156.80	151.0
158.80	133.0
160.70	137.0
171.70	336.0
172.90	785.0
173.80	92920.0
174.80	6944.0
175.80	90728.0
176.80	5773.0
177.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	793.0
36.90	4770.0
37.90	4717.0
38.90	1747.0
39.80	273.0
43.90	1008.0
44.90	902.0
46.90	1154.0
47.80	686.0
48.90	4642.0
49.90	20928.0
50.90	6528.0
51.90	343.0
54.90	382.0
55.90	1818.0
56.90	3460.0
59.90	1071.0
60.90	5756.0
61.90	4904.0
63.00	4260.0
64.00	366.0
64.90	180.0
67.00	365.0
67.90	12335.0
68.90	11757.0
69.90	937.0
71.80	548.0
72.90	5146.0
73.90	20216.0
74.90	60552.0
75.90	4880.0
76.90	818.0
77.80	492.0
78.80	4148.0
79.80	1233.0
80.80	4345.0
81.80	886.0
83.00	144.0
86.90	4632.0
87.90	4531.0
90.80	431.0
91.90	3542.0
92.90	5074.0
93.90	13468.0
94.90	114416.0
95.90	7264.0
96.90	185.0
103.90	555.0
104.80	225.0
105.80	558.0
106.70	126.0
112.80	154.0
114.80	139.0
115.80	523.0
116.80	648.0
117.80	472.0
118.80	588.0
127.80	336.0
128.80	236.0
129.70	379.0
130.60	102.0
134.70	240.0
136.70	169.0
139.80	108.0
140.80	1181.0
141.70	145.0
142.80	1249.0
144.90	114.0
145.80	206.0
147.80	223.0
149.70	104.0
153.80	104.0
154.80	279.0
156.80	143.0
158.80	118.0
160.80	181.0
171.70	378.0
172.80	814.0
173.80	88400.0
174.80	6479.0
175.80	86328.0
176.80	5452.0
177.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013