


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102424\
Data File : VU061194.D
Acq On : 24 Oct 2024 09:23
Operator : MD/SY
Sample : BFB014
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB014

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 25 02:35:03 2024

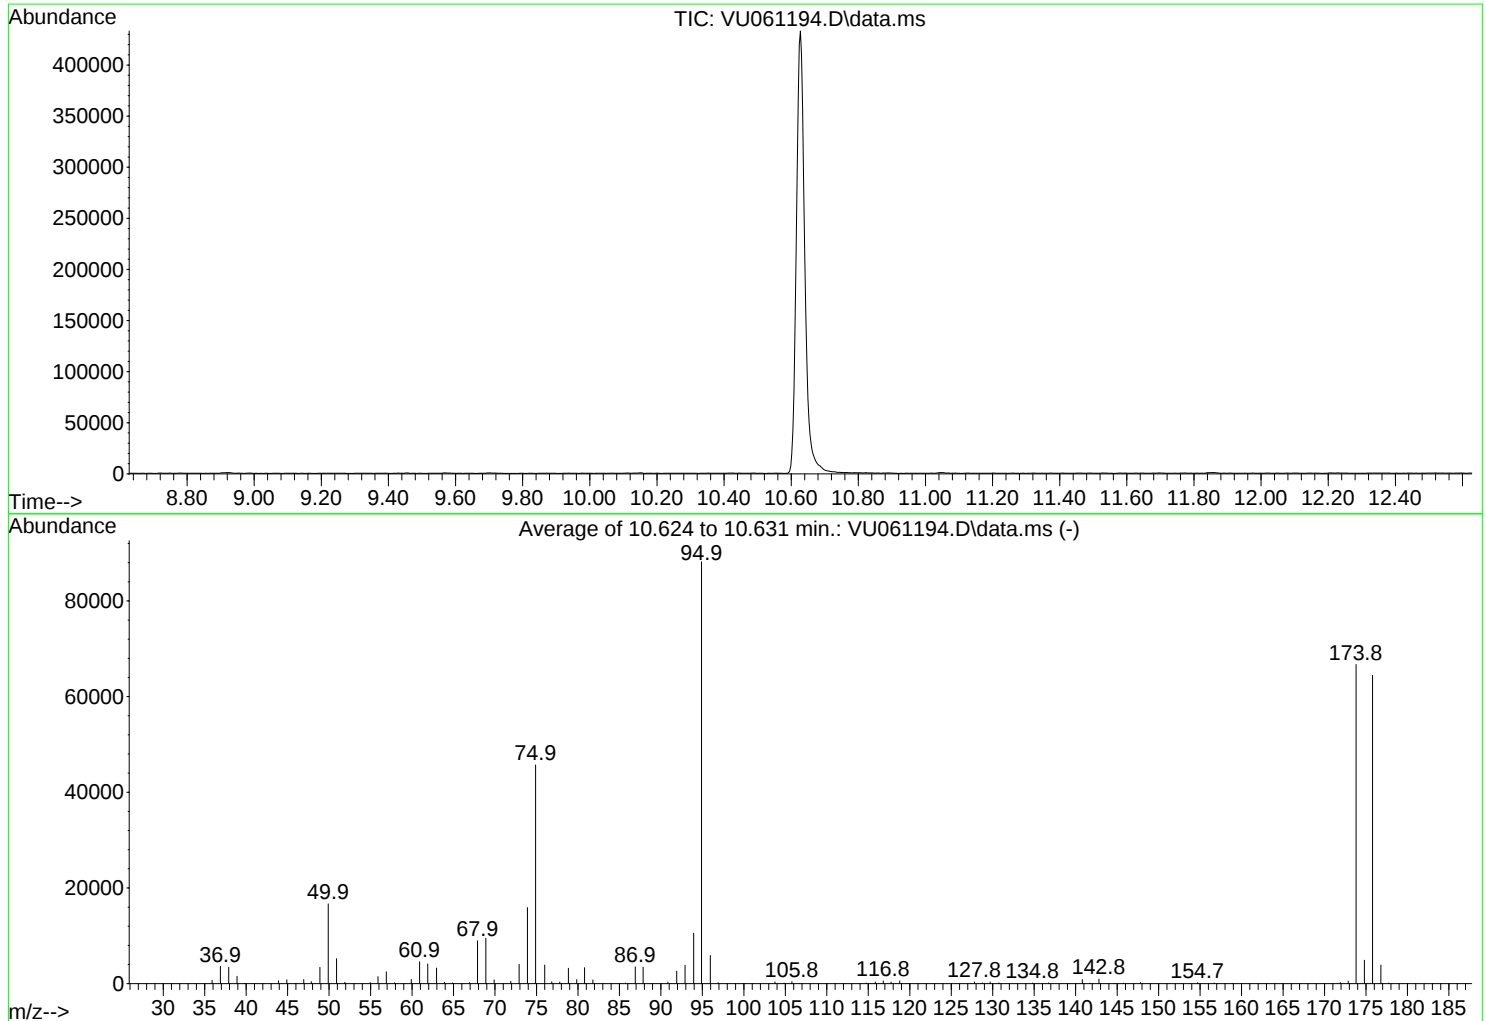

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	16693	PASS
75	95	30	80	51.9	45728	PASS
95	95	100	100	100.0	88173	PASS
96	95	5	9	6.7	5882	PASS
173	174	0.00	2	0.8	537	PASS
174	95	50	120	75.7	66717	PASS
175	174	5	9	7.3	4902	PASS
176	174	95	101	96.6	64448	PASS
177	176	5	9	6.0	3895	PASS

Scan 2890 (10.582 min): VU061194.D\data.ms
BFB014

m/z	Abundance
39.70	196.0
43.90	322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	754.0
36.90	3566.0
37.90	3431.0
38.90	1588.0
39.90	285.0
43.90	936.0
44.90	861.0
46.00	123.0
46.90	826.0
47.90	411.0
48.90	3469.0
49.90	17008.0
50.90	5223.0
51.90	300.0
55.00	252.0
55.90	1481.0
56.90	2508.0
57.90	168.0
59.90	828.0
60.90	4736.0
61.90	4121.0
63.00	3144.0
63.90	324.0
64.90	155.0
67.00	190.0
67.90	9051.0
68.90	9489.0
69.90	790.0
71.90	543.0
72.90	4200.0
73.90	15762.0
74.90	46200.0
76.00	3973.0
76.80	461.0
77.80	356.0
78.90	3179.0
79.90	806.0
80.80	3316.0
81.80	751.0
85.70	150.0
86.90	3358.0
87.90	3612.0
90.90	351.0
91.90	2519.0
92.90	3866.0
94.00	10935.0
94.90	88096.0
96.00	6036.0
96.90	238.0
103.70	404.0
104.80	147.0
105.80	374.0
114.70	152.0
115.80	439.0
116.80	619.0
117.80	301.0
118.80	559.0
127.80	301.0
128.70	173.0
129.70	335.0
130.70	135.0
134.80	114.0
136.80	167.0
140.80	810.0
141.70	108.0
142.80	985.0
145.80	121.0
147.80	245.0
154.70	165.0
156.70	112.0
172.00	254.0
172.80	507.0
173.80	65264.0
174.80	4871.0
175.80	63280.0
176.80	3978.0
177.80	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	719.0
36.90	3711.0
37.90	3499.0
38.90	1585.0
39.90	279.0
43.90	929.0
44.90	842.0
46.00	120.0
47.00	875.0
47.80	434.0
48.90	3497.0
49.90	17200.0
50.90	5396.0
51.90	322.0
54.90	218.0
55.90	1526.0
56.90	2521.0
57.90	194.0
59.90	894.0
60.90	4797.0
61.90	4191.0
63.00	3293.0
63.90	309.0
64.90	183.0
67.00	186.0
67.90	9232.0
68.90	9749.0
69.90	792.0
71.90	521.0
72.90	4119.0
73.90	16299.0
74.90	46984.0
76.00	3979.0
76.90	406.0
77.80	360.0
78.80	3307.0
79.90	886.0
80.80	3374.0
81.80	797.0
85.80	154.0
86.90	3658.0
87.80	3545.0
90.90	365.0
91.90	2673.0
92.90	3944.0
93.90	10819.0
94.90	91032.0
96.00	6040.0
96.90	223.0
103.80	380.0
104.80	158.0
105.80	449.0
106.70	106.0
114.80	143.0
115.90	383.0
116.80	583.0
117.70	360.0
118.80	603.0
127.80	396.0
128.70	156.0
129.70	386.0
130.70	160.0
134.80	125.0
136.70	152.0
140.80	842.0
141.70	100.0
142.80	1009.0
144.70	101.0
145.80	155.0
147.80	244.0
154.70	213.0
156.70	132.0
171.90	227.0
172.90	563.0
173.80	68672.0
174.80	5045.0
175.80	66296.0
176.80	3960.0
177.70	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	596.0
36.90	3545.0
37.90	3295.0
38.90	1445.0
39.90	274.0
43.90	913.0
44.90	718.0
46.90	872.0
47.80	416.0
48.90	3272.0
49.90	15872.0
50.90	5050.0
51.90	266.0
54.90	229.0
55.90	1403.0
56.90	2403.0
57.90	170.0
59.90	906.0
60.90	4260.0
61.90	3987.0
62.90	3259.0
63.90	260.0
64.90	160.0
66.90	189.0
67.90	8601.0
68.90	9246.0
69.90	704.0
71.90	444.0
72.90	3821.0
73.90	15562.0
74.90	44000.0
76.00	3693.0
76.90	390.0
77.80	335.0
78.80	3140.0
79.80	872.0
80.80	3327.0
81.80	781.0
85.80	118.0
86.90	3558.0
87.80	3214.0
90.80	306.0
91.90	2632.0
92.90	3717.0
93.90	9809.0
94.90	85392.0
95.90	5569.0
96.90	195.0
103.80	356.0
104.90	145.0
105.80	486.0
114.80	129.0
115.90	308.0
116.80	554.0
117.70	387.0
118.80	553.0
127.80	389.0
128.80	132.0
129.70	364.0
130.80	162.0
134.80	137.0
136.70	153.0
140.80	849.0
141.70	109.0
142.80	943.0
145.80	145.0
147.80	216.0
154.70	205.0
156.70	147.0
158.90	113.0
171.80	205.0
172.90	542.0
173.80	66216.0
174.80	4790.0
175.80	63768.0
176.80	3747.0
177.70	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014