
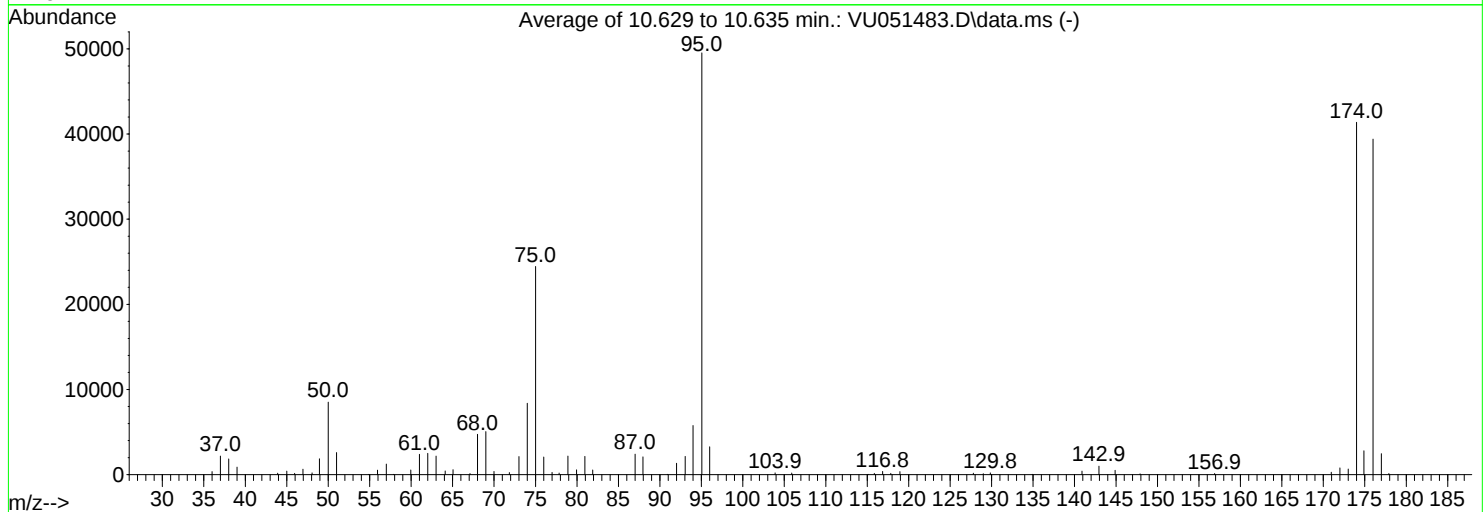


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102522\
 Data File : VU051483.D
 Acq On : 25 Oct 2022 10:59
 Operator : JC/MD
 Sample : BFB140
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB140

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 27 01:27:49 2022

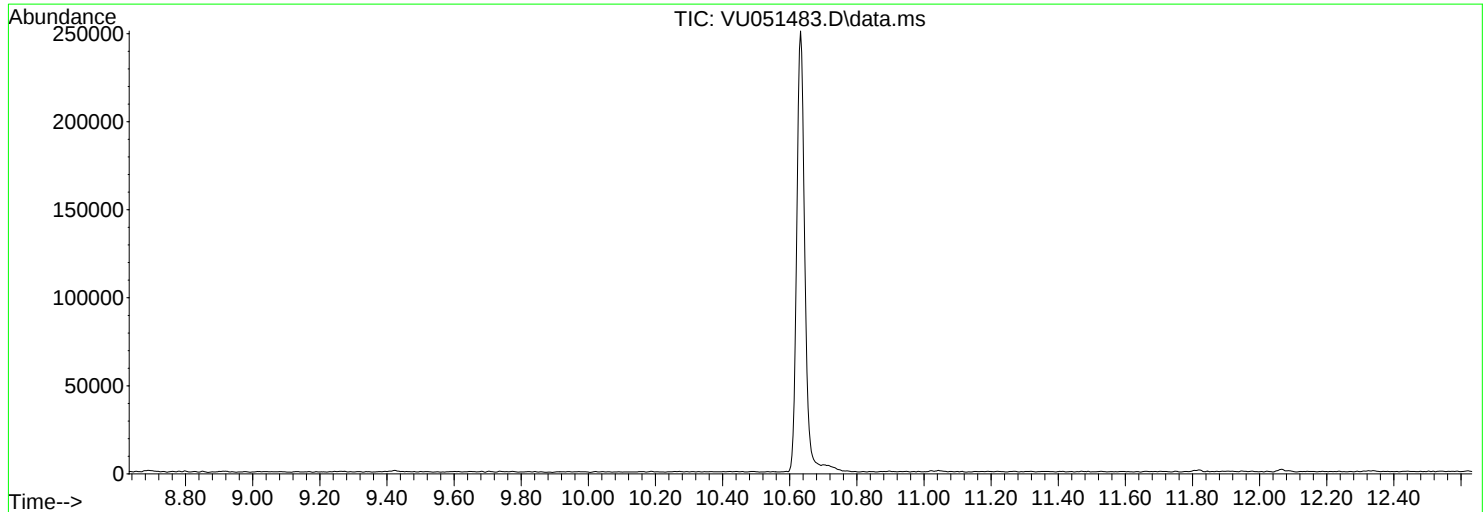

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8523	PASS
75	95	30	80	49.4	24451	PASS
95	95	100	100	100.0	49536	PASS
96	95	5	9	6.6	3266	PASS
173	174	0.00	2	1.6	667	PASS
174	95	50	120	83.5	41368	PASS
175	174	5	9	6.8	2798	PASS
176	174	95	101	95.3	39413	PASS
177	176	5	9	6.3	2466	PASS

m/z	Abundance
39.90	397.0
44.00	1023.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
36.00	343.0
37.00	2428.0
38.00	1952.0
39.00	951.0
40.00	371.0
43.90	1219.0
45.00	417.0
46.00	170.0
46.90	628.0
48.10	214.0
49.00	1805.0
50.00	8609.0
51.00	2461.0
56.00	538.0
57.00	1300.0
60.00	543.0
61.00	2480.0
62.00	2504.0
63.00	2219.0
64.10	432.0
65.10	596.0
67.10	135.0
68.00	4758.0
69.00	4919.0
70.00	403.0
71.80	169.0
73.00	2047.0
74.00	8468.0
75.00	24576.0
76.00	2169.0
77.00	277.0
77.80	181.0
78.90	2054.0
80.00	537.0
81.00	2089.0
81.90	565.0
87.00	2262.0
88.00	2116.0
92.00	1333.0
93.10	2037.0
94.00	5851.0
95.00	49000.0
96.00	3393.0
103.90	224.0
105.90	220.0
115.10	113.0
115.90	135.0
116.90	353.0
117.80	173.0
119.00	363.0
127.80	183.0
129.00	120.0
129.80	210.0
134.90	105.0
140.90	376.0
142.90	989.0
144.90	459.0
156.90	131.0
170.90	280.0
172.00	830.0
173.00	622.0
174.00	40112.0
174.90	2875.0
176.00	37624.0
177.00	2613.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
36.00	371.0
37.00	2231.0
38.00	1945.0
39.00	928.0
40.00	369.0
43.90	1181.0
45.00	418.0
46.00	132.0
46.90	693.0
48.00	209.0
48.90	1926.0
50.00	8807.0
51.00	2682.0
55.90	526.0
57.00	1276.0
60.00	545.0
61.00	2472.0
62.00	2583.0
63.00	2250.0
64.10	417.0
65.10	608.0
67.10	161.0
68.00	4861.0
69.00	5183.0
70.00	399.0
71.90	249.0
73.00	2249.0
74.00	8667.0
75.00	25312.0
76.00	2109.0
77.00	280.0
77.90	199.0
78.90	2200.0
80.00	577.0
81.00	2170.0
81.90	570.0
87.00	2532.0
87.90	2124.0
92.00	1388.0
93.00	2201.0
94.00	5994.0
95.10	51120.0
96.00	3357.0
103.90	216.0
105.90	204.0
115.80	145.0
116.90	369.0
117.90	153.0
118.90	362.0
127.80	167.0
129.00	125.0
129.90	220.0
140.90	425.0
142.90	1055.0
144.90	546.0
147.90	121.0
156.90	145.0
171.00	295.0
172.00	812.0
173.00	696.0
174.00	42664.0
174.90	2822.0
176.00	40800.0
177.00	2508.0
177.90	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
36.00	363.0
37.00	1878.0
38.00	1654.0
39.00	794.0
40.00	378.0
43.90	1162.0
45.00	407.0
45.90	134.0
47.00	605.0
48.00	202.0
49.00	1828.0
50.00	8152.0
51.00	2664.0
54.90	125.0
55.90	492.0
57.00	1172.0
57.90	122.0
59.90	546.0
61.00	2192.0
62.00	2436.0
63.00	2082.0
64.10	426.0
65.00	563.0
67.10	125.0
68.00	4564.0
69.00	5068.0
70.00	348.0
71.90	334.0
73.00	2103.0
74.00	8033.0
75.00	23464.0
76.00	1911.0
77.00	248.0
77.90	169.0
78.90	2279.0
79.90	593.0
80.90	2177.0
81.90	485.0
87.00	2439.0
87.90	2010.0
90.90	105.0
92.00	1315.0
93.00	2203.0
94.00	5481.0
95.10	48488.0
96.00	3049.0
103.90	196.0
105.90	152.0
115.80	161.0
116.80	382.0
117.80	136.0
118.90	352.0
127.80	141.0
129.00	101.0
129.90	178.0
140.90	435.0
143.00	967.0
144.90	513.0
147.90	150.0
156.90	113.0
171.00	286.0
172.00	711.0
173.00	682.0
174.00	41328.0
174.90	2696.0
176.00	39816.0
177.00	2276.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140