

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
 Data File : VU061239.D
 Acq On : 25 Oct 2024 21:06
 Operator : MD/SY
 Sample : P4560-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCNX9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	116	rBV	68537	81322	13.67%	1.558%
2	1.911	180	193	208	rBV	63203	88890	14.94%	1.703%
3	2.364	327	334	345	rVB6	3370	6265	1.05%	0.120%
4	2.560	384	395	413	rBV	121704	200074	33.64%	3.834%
5	3.358	632	643	657	rBV2	4211	9403	1.58%	0.180%
6	3.862	785	800	820	rVB3	8121	20187	3.39%	0.387%
7	4.631	1024	1039	1065	rBV2	73166	206461	34.71%	3.956%
8	5.055	1156	1171	1190	rBV	109419	248521	41.78%	4.762%
9	5.718	1357	1377	1404	rBV2	228103	594834	100.00%	11.399%
10	6.242	1526	1540	1563	rBV	222879	431130	72.48%	8.262%
11	6.541	1623	1633	1647	rBV3	17397	32966	5.54%	0.632%
12	6.682	1665	1677	1704	rBV	134392	269969	45.39%	5.173%
13	7.560	1939	1950	1983	rBV	69715	131865	22.17%	2.527%
14	7.891	2040	2053	2082	rBV	288223	519419	87.32%	9.954%
15	8.177	2127	2142	2162	rBV	38761	72791	12.24%	1.395%
16	8.547	2244	2257	2272	rBV2	92383	159765	26.86%	3.062%
17	8.631	2272	2283	2322	rVV2	274631	573229	96.37%	10.985%
18	9.412	2514	2526	2553	rBV	302883	527349	88.65%	10.106%
19	10.750	2931	2942	2961	rBV	96289	162078	27.25%	3.106%
20	11.807	3260	3271	3297	rBV	283337	473672	79.63%	9.077%
21	12.187	3375	3389	3409	rBV	242447	408198	68.62%	7.822%




Sum of corrected areas: 5218388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061239.D
Acq On : 25 Oct 2024 21:06
Operator : MD/SY
Sample : P4560-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

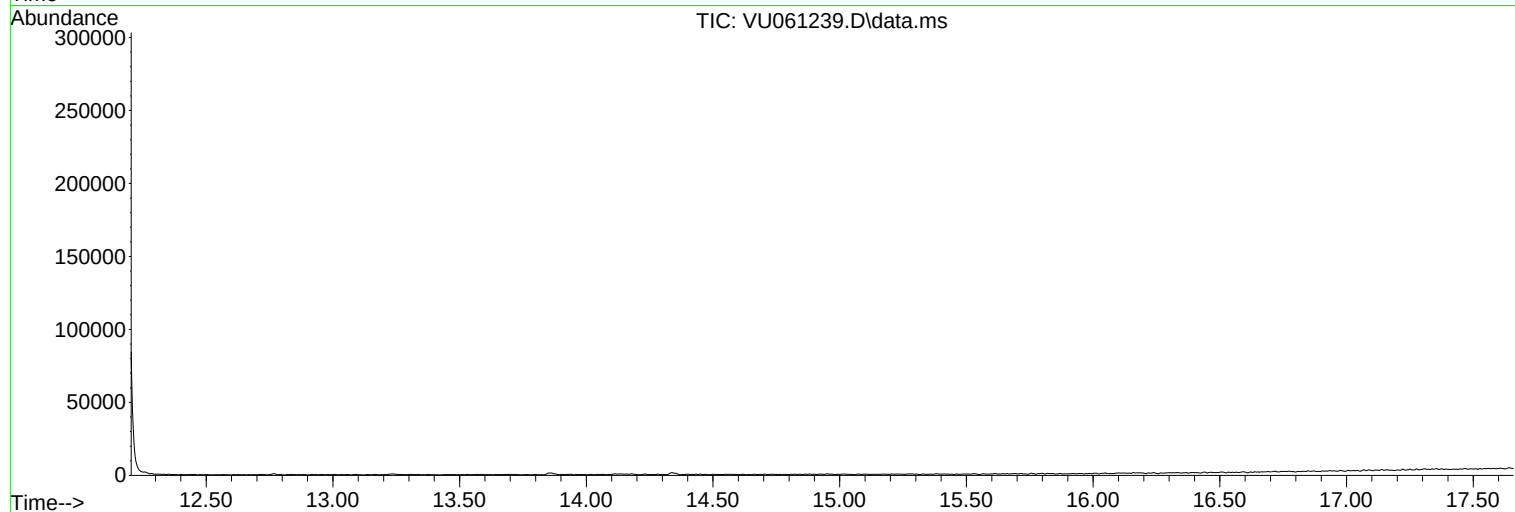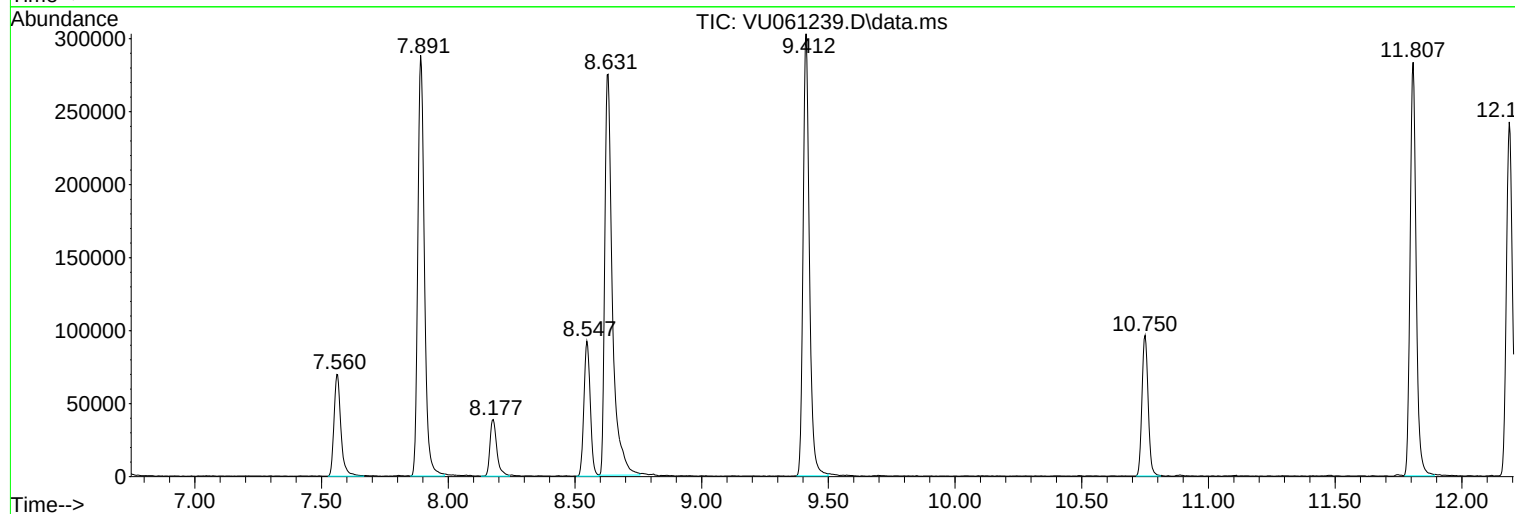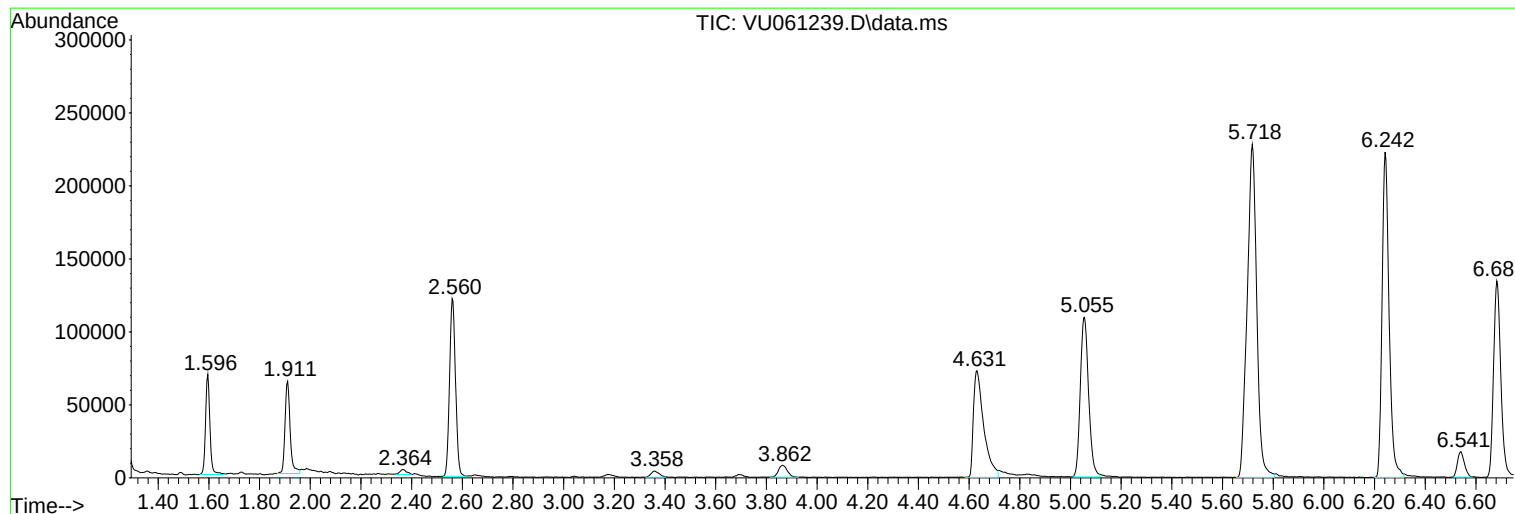

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061239.D
Acq On : 25 Oct 2024 21:06
Operator : MD/SY
Sample : P4560-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061239.D
Acq On : 25 Oct 2024 21:06
Operator : MD/SY
Sample : P4560-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc