

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
 Data File : VU061240.D
 Acq On : 25 Oct 2024 21:30
 Operator : MD/SY
 Sample : P4560-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCNY0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU061240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rVB	69884	81622	13.37%	1.543%
2	1.908	184	192	207	rBV	66491	92402	15.13%	1.746%
3	2.560	383	395	412	rBV	120803	198304	32.48%	3.748%
4	3.171	575	585	605	rVB2	2556	6581	1.08%	0.124%
5	3.354	623	642	669	rBV2	87860	208490	34.15%	3.941%
6	4.628	1024	1038	1080	rBV	78546	223704	36.64%	4.228%
7	5.055	1152	1171	1206	rBV	114938	262926	43.06%	4.970%
8	5.718	1358	1377	1407	rBV2	232491	610543	100.00%	11.540%
9	6.242	1528	1540	1567	rBV	216996	429414	70.33%	8.116%
10	6.682	1663	1677	1698	rBV	137497	277444	45.44%	5.244%
11	7.560	1938	1950	1975	rBV	71437	132303	21.67%	2.501%
12	7.891	2040	2053	2080	rBV	287073	522359	85.56%	9.873%
13	8.177	2127	2142	2166	rBV	39812	73882	12.10%	1.396%
14	8.628	2271	2282	2321	rBV	293165	602104	98.62%	11.380%
15	9.409	2511	2525	2559	rBV	290231	518520	84.93%	9.801%
16	10.746	2927	2941	2962	rBV	100400	167573	27.45%	3.167%
17	11.807	3259	3271	3304	rBV	273197	462484	75.75%	8.741%
18	12.068	3340	3352	3373	rBV5	4801	12989	2.13%	0.246%
19	12.187	3377	3389	3420	rVB	238611	407076	66.67%	7.694%




Sum of corrected areas: 5290720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061240.D
Acq On : 25 Oct 2024 21:30
Operator : MD/SY
Sample : P4560-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

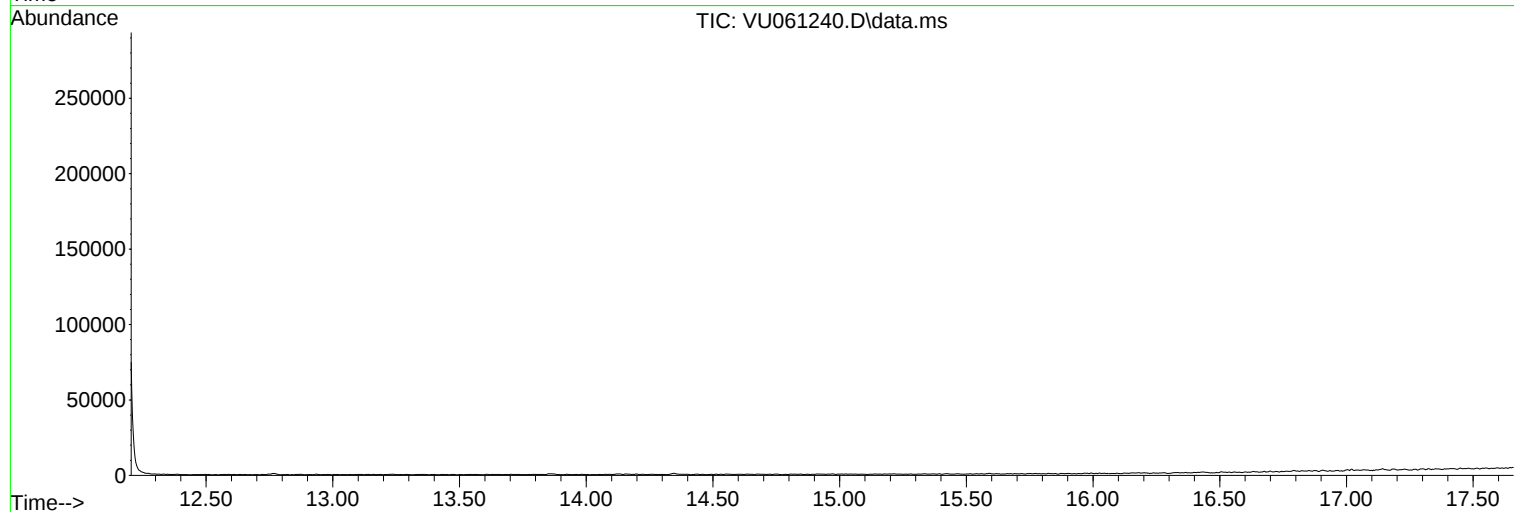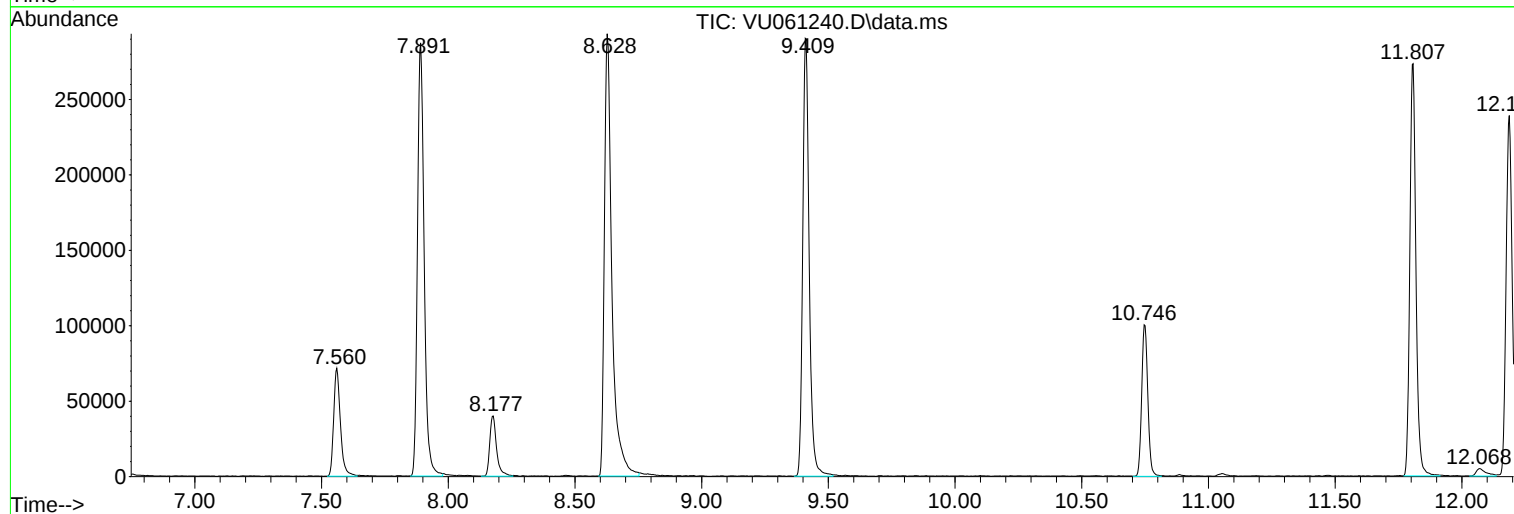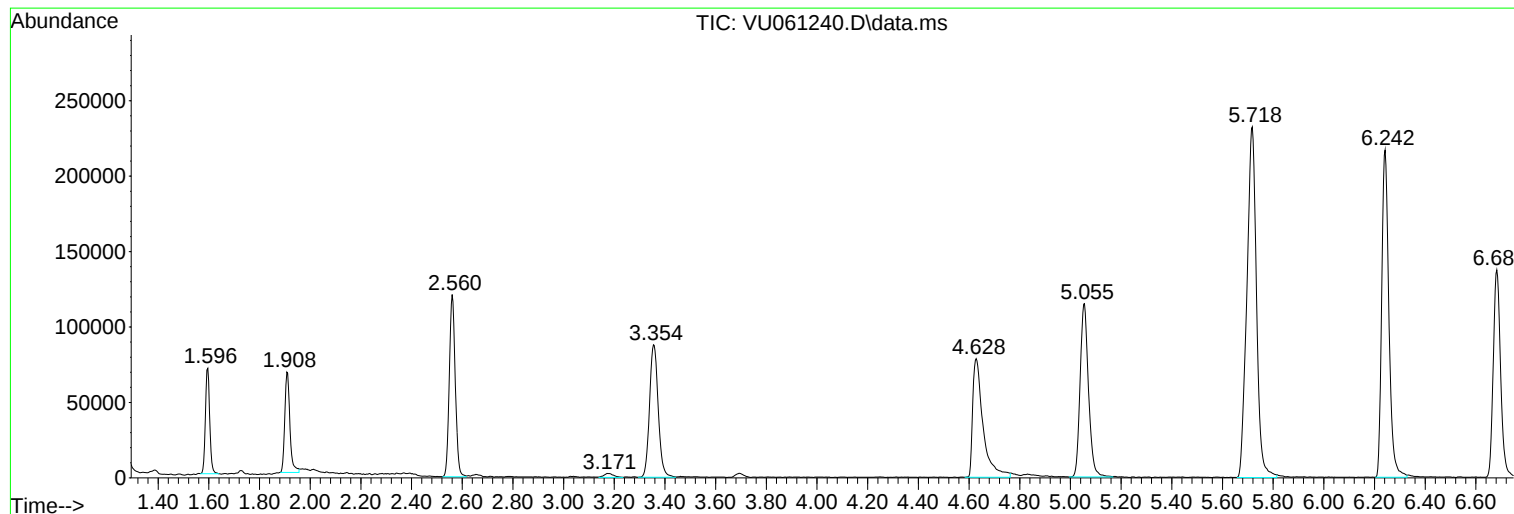

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061240.D
Acq On : 25 Oct 2024 21:30
Operator : MD/SY
Sample : P4560-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061240.D
Acq On : 25 Oct 2024 21:30
Operator : MD/SY
Sample : P4560-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc