

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
 Data File : VU061252.D
 Acq On : 26 Oct 2024 02:24
 Operator : MD/SY
 Sample : P4560-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCNZ2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU061252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	105	rBV	63806	72706	13.15%	1.542%
2	1.911	184	193	203	rBV	59901	80023	14.47%	1.697%
3	2.560	383	395	413	rBV	108511	177635	32.12%	3.768%
4	3.181	576	588	601	rVB2	2540	5996	1.08%	0.127%
5	3.354	628	642	663	rBV2	47543	110158	19.92%	2.337%
6	3.695	736	748	760	rBV4	2337	5559	1.01%	0.118%
7	4.631	1025	1039	1065	rBV	68610	187010	33.81%	3.967%
8	5.052	1155	1170	1196	rBV2	102621	234624	42.42%	4.977%
9	5.718	1358	1377	1405	rBV2	213564	553106	100.00%	11.732%
10	6.242	1527	1540	1571	rBV	214123	415238	75.07%	8.808%
11	6.682	1664	1677	1707	rBV	127419	253816	45.89%	5.384%
12	7.560	1939	1950	1968	rBV	62512	115915	20.96%	2.459%
13	7.891	2040	2053	2076	rBV	259613	467684	84.56%	9.920%
14	8.174	2130	2141	2162	rBV	34546	63108	11.41%	1.339%
15	8.627	2271	2282	2317	rBV	256895	525196	94.95%	11.140%
16	9.412	2512	2526	2560	rBV	286004	501784	90.72%	10.643%
17	10.749	2930	2942	2961	rBV	89217	147898	26.74%	3.137%
18	11.804	3259	3270	3298	rBV	261850	436202	78.86%	9.252%
19	12.187	3377	3389	3409	rBV	213709	360810	65.23%	7.653%




Sum of corrected areas: 4714468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061252.D
Acq On : 26 Oct 2024 02:24
Operator : MD/SY
Sample : P4560-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

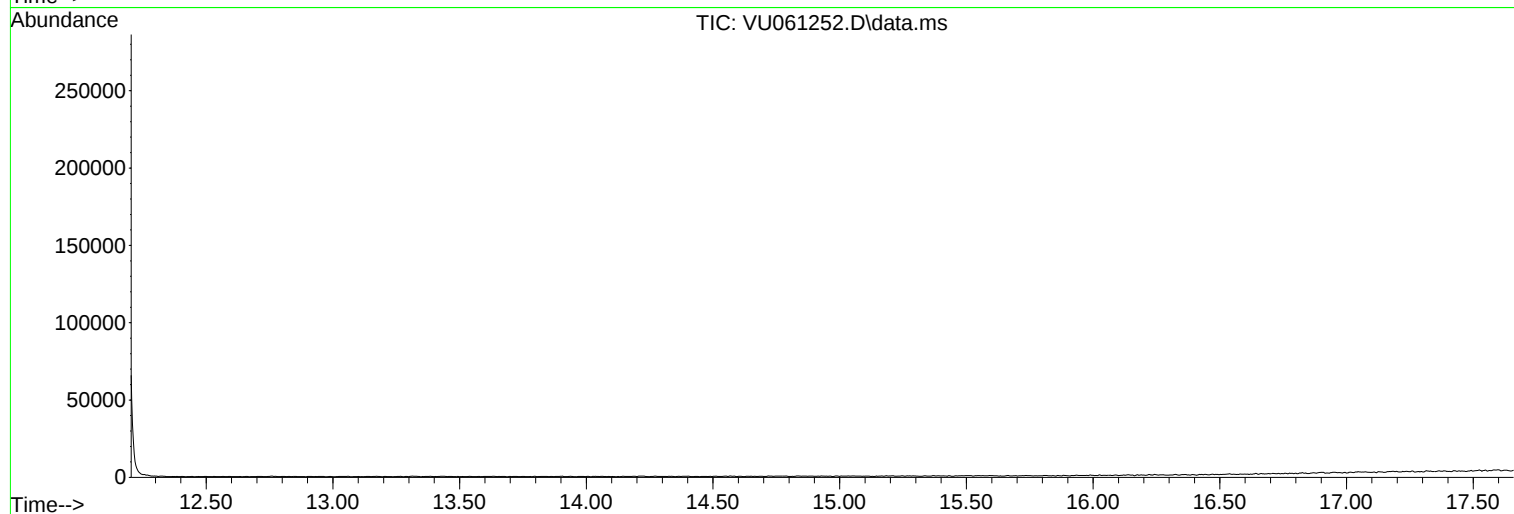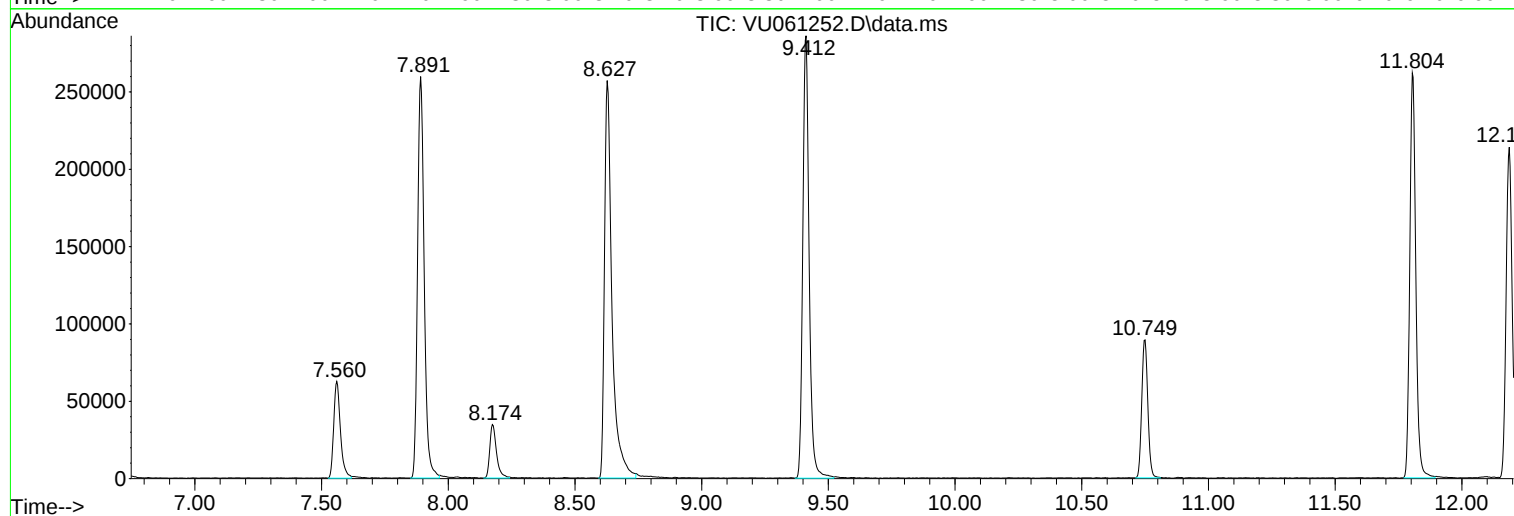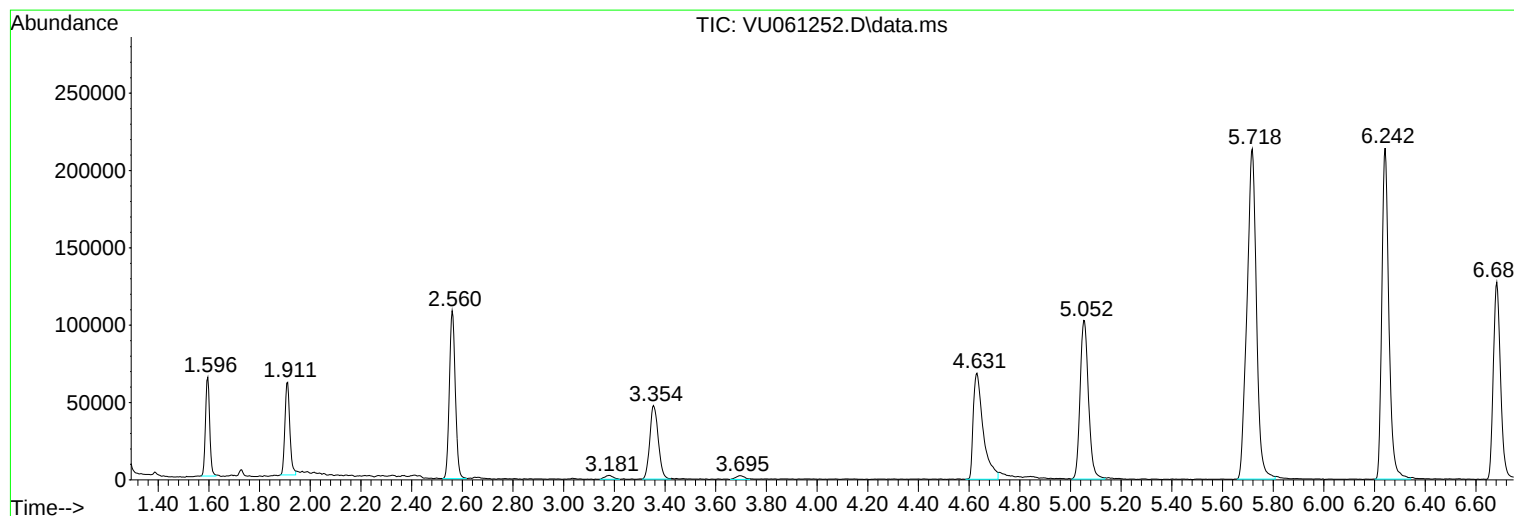

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061252.D
Acq On : 26 Oct 2024 02:24
Operator : MD/SY
Sample : P4560-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061252.D
Acq On : 26 Oct 2024 02:24
Operator : MD/SY
Sample : P4560-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc