

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
 Data File : VU061254.D
 Acq On : 26 Oct 2024 03:13
 Operator : MD/SY
 Sample : P4560-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCNZ4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU061254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	109	rBV	68026	76857	13.52%	1.581%
2	1.911	184	193	206	rBV	59574	83103	14.62%	1.710%
3	2.560	383	395	413	rBV	105827	173754	30.58%	3.575%
4	3.357	627	643	663	rBV2	61336	143177	25.20%	2.946%
5	4.631	1029	1039	1067	rBV	70037	194327	34.20%	3.998%
6	5.055	1155	1171	1192	rBV	105608	238013	41.88%	4.897%
7	5.718	1358	1377	1405	rBV2	217692	568263	100.00%	11.692%
8	6.242	1527	1540	1574	rBV	211927	415819	73.17%	8.555%
9	6.544	1625	1634	1646	rVB4	4457	7742	1.36%	0.159%
10	6.682	1664	1677	1701	rBV	132521	263343	46.34%	5.418%
11	7.560	1939	1950	1973	rBV	64326	118772	20.90%	2.444%
12	7.891	2040	2053	2083	rBV	266647	483984	85.17%	9.958%
13	8.174	2131	2141	2169	rBV	36860	67751	11.92%	1.394%
14	8.627	2271	2282	2312	rBV2	263184	541898	95.36%	11.149%
15	9.409	2514	2525	2549	rBV	288749	499165	87.84%	10.270%
16	10.749	2927	2942	2963	rBV	93417	154204	27.14%	3.173%
17	11.804	3258	3270	3298	rBV	258864	438793	77.22%	9.028%
18	12.068	3342	3352	3364	rBV5	6454	15370	2.70%	0.316%
19	12.187	3377	3389	3410	rBV	222821	376090	66.18%	7.738%




Sum of corrected areas: 4860425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061254.D
Acq On : 26 Oct 2024 03:13
Operator : MD/SY
Sample : P4560-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

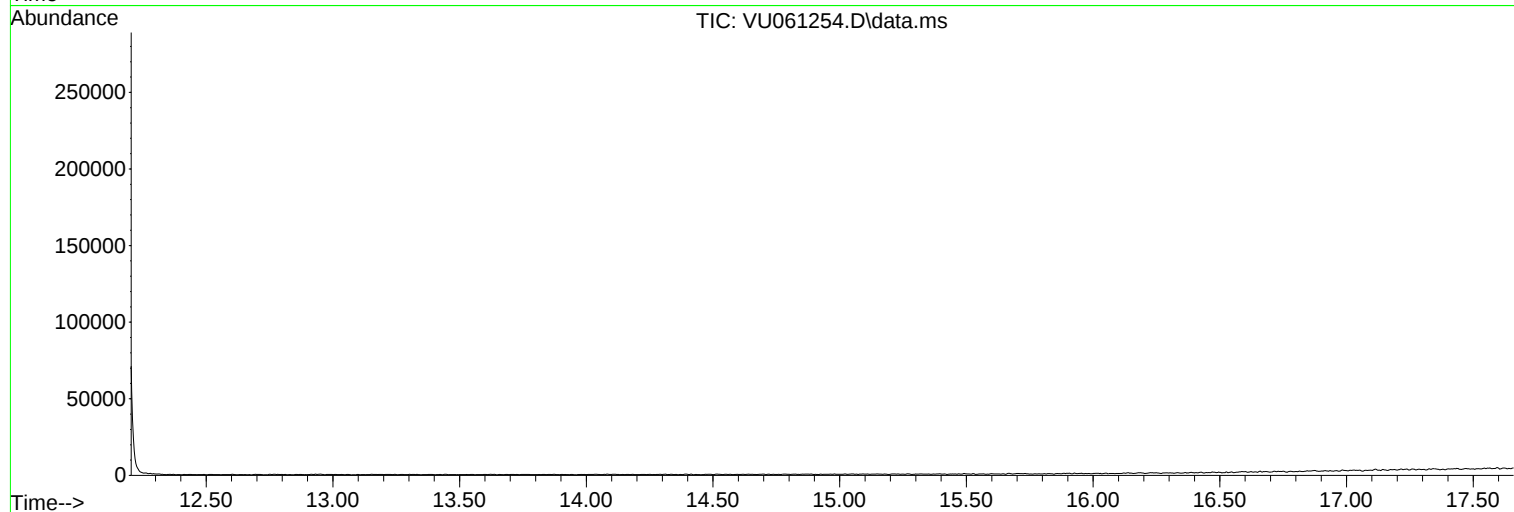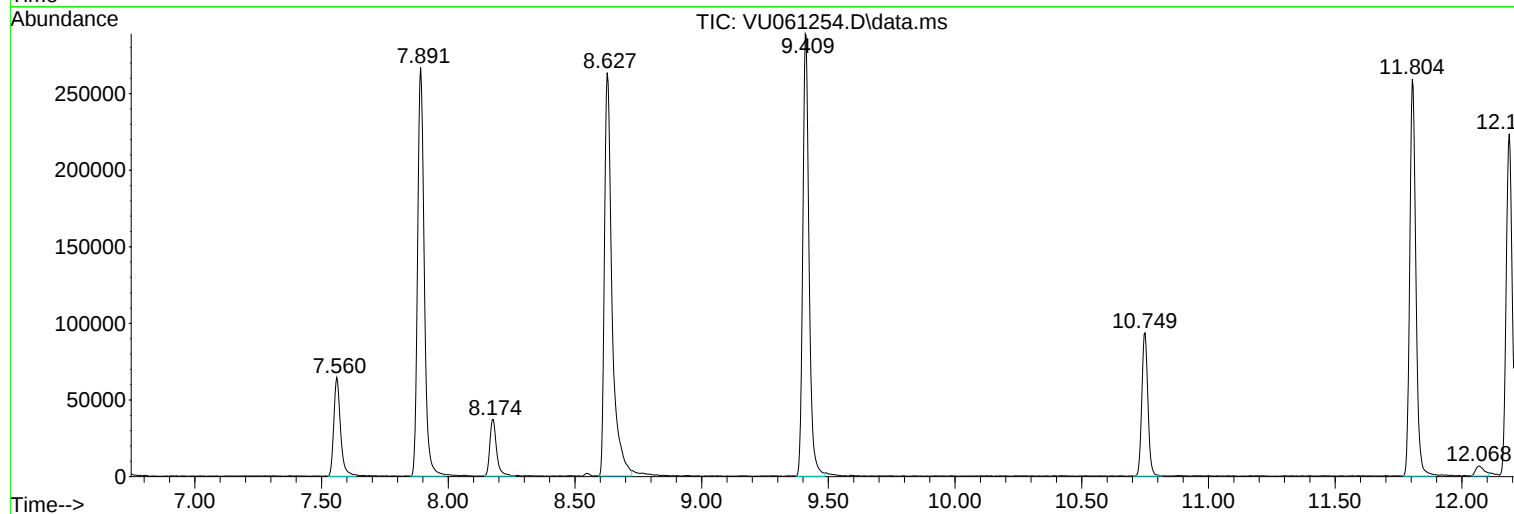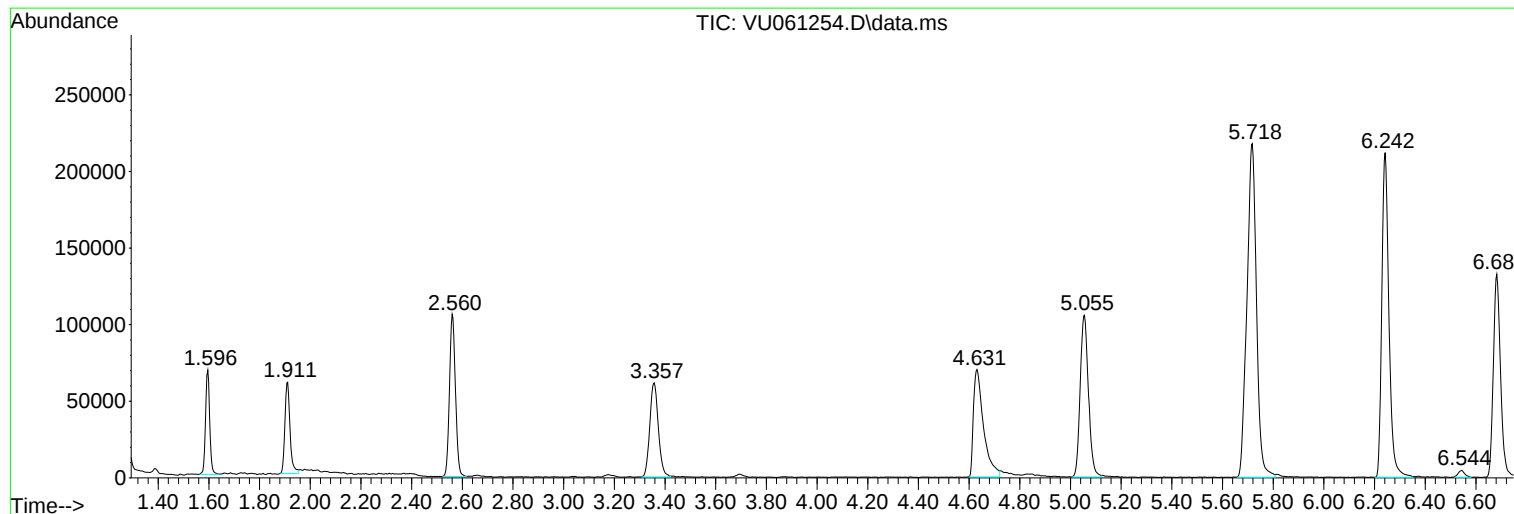

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061254.D
Acq On : 26 Oct 2024 03:13
Operator : MD/SY
Sample : P4560-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061254.D
Acq On : 26 Oct 2024 03:13
Operator : MD/SY
Sample : P4560-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCNZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
