


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102524\
Data File : VU061213.D
Acq On : 25 Oct 2024 08:37
Operator : MD/SY
Sample : BFB015
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB015

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Oct 26 01:22:04 2024

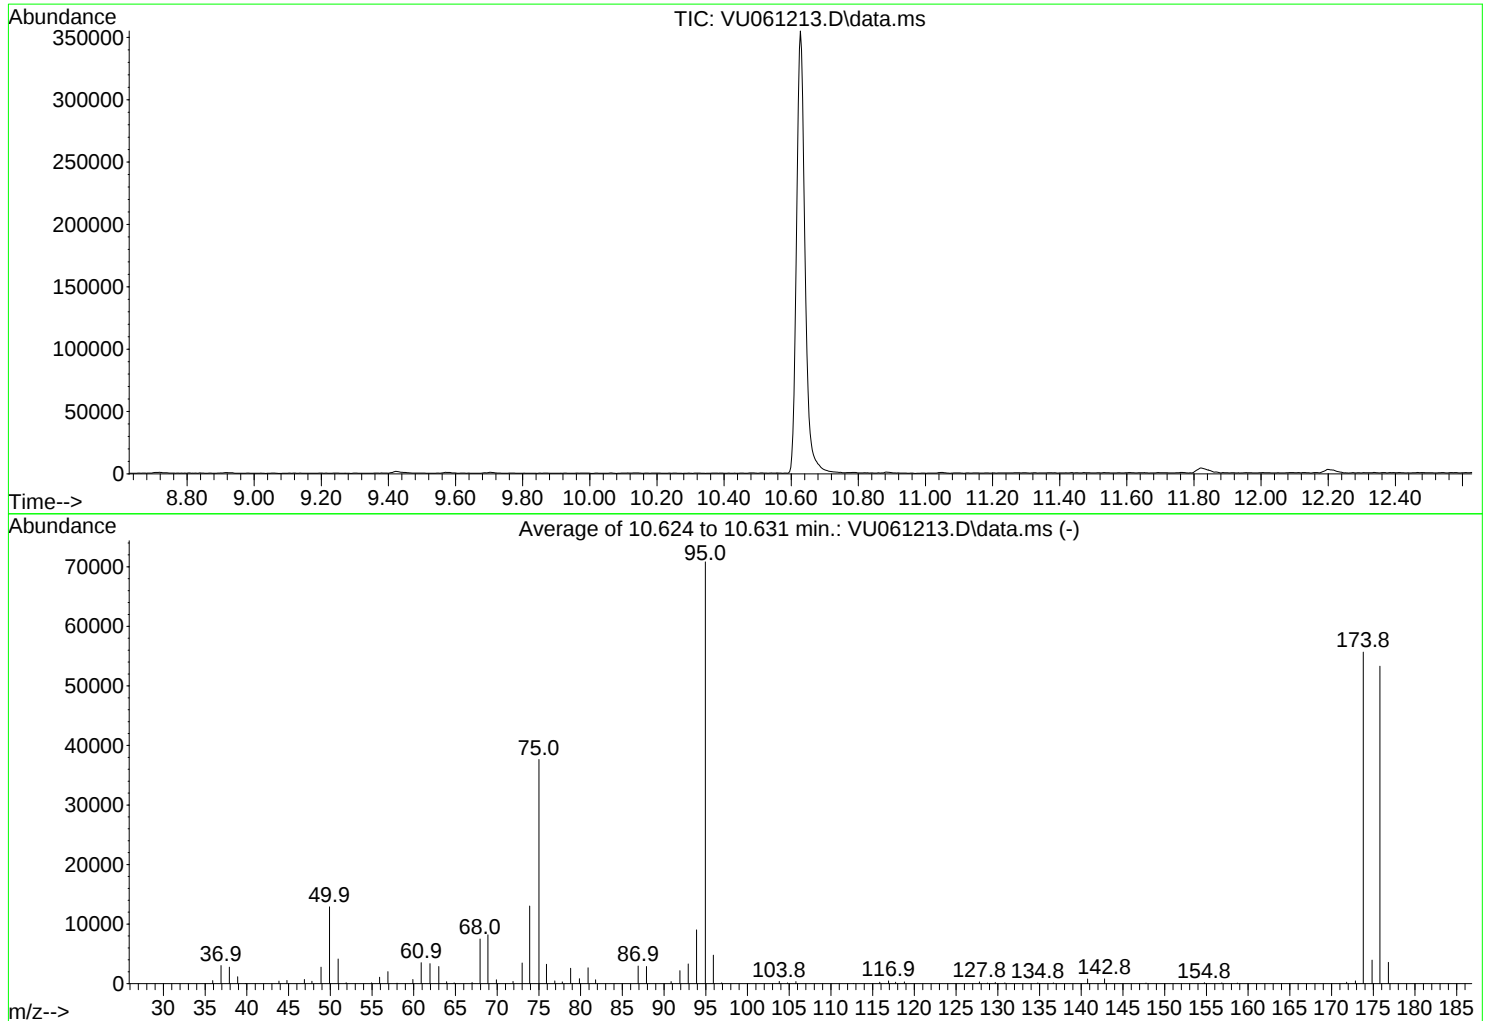

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	12895	PASS
75	95	30	80	53.2	37653	PASS
95	95	100	100	100.0	70837	PASS
96	95	5	9	6.7	4777	PASS
173	174	0.00	2	0.8	452	PASS
174	95	50	120	78.6	55675	PASS
175	174	5	9	7.1	3959	PASS
176	174	95	101	95.7	53301	PASS
177	176	5	9	6.7	3568	PASS

m/z	Abundance
39.80	250.0
43.80	389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	519.0
36.90	2953.0
37.90	2831.0
38.90	1112.0
39.90	311.0
43.90	803.0
44.80	564.0
46.90	772.0
47.80	483.0
48.90	2771.0
49.90	13177.0
50.90	4072.0
51.90	175.0
54.90	136.0
55.90	1119.0
56.90	1971.0
59.90	706.0
60.90	3541.0
61.90	3404.0
63.00	3084.0
63.90	310.0
65.00	154.0
67.00	185.0
68.00	7563.0
68.90	8242.0
69.90	670.0
71.90	360.0
73.00	3518.0
73.90	13297.0
75.00	37488.0
75.90	3237.0
76.90	513.0
77.80	322.0
78.80	2574.0
79.90	850.0
80.90	2635.0
81.80	608.0
86.90	3012.0
87.90	2893.0
90.90	313.0
91.90	2082.0
92.90	3230.0
93.90	8856.0
95.00	69792.0
95.90	4701.0
96.90	141.0
103.80	344.0
104.80	124.0
105.80	348.0
115.80	264.0
116.90	439.0
117.80	218.0
118.80	344.0
127.80	261.0
128.80	115.0
129.70	190.0
130.80	136.0
134.70	165.0
136.70	158.0
140.80	770.0
142.80	805.0
147.70	120.0
154.80	152.0
156.90	120.0
171.80	227.0
172.80	463.0
173.80	53488.0
174.90	3848.0
175.80	51800.0
176.80	3590.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	518.0
36.90	3139.0
37.90	2845.0
38.90	1190.0
39.90	301.0
43.90	808.0
44.80	534.0
46.90	753.0
47.80	413.0
48.90	2877.0
49.90	13232.0
50.90	4282.0
51.90	181.0
55.00	133.0
55.90	1103.0
56.90	2048.0
58.00	118.0
59.90	692.0
60.90	3631.0
61.90	3422.0
63.00	2949.0
63.90	346.0
64.80	129.0
67.00	210.0
67.90	7688.0
68.90	8487.0
69.90	694.0
71.90	374.0
73.00	3686.0
73.90	13379.0
75.00	38672.0
75.90	3337.0
76.90	482.0
77.80	329.0
78.80	2656.0
79.80	847.0
80.90	2763.0
81.80	677.0
86.90	3108.0
87.90	2947.0
90.80	350.0
91.90	2251.0
92.90	3347.0
93.90	9238.0
94.90	72704.0
95.90	4887.0
96.90	131.0
103.80	397.0
104.80	135.0
105.80	372.0
115.90	247.0
116.90	461.0
117.80	260.0
118.80	322.0
127.80	310.0
128.70	119.0
129.70	219.0
130.90	151.0
134.80	133.0
136.70	149.0
140.80	773.0
142.80	826.0
147.70	124.0
154.80	183.0
156.80	135.0
158.70	145.0
171.80	272.0
172.80	455.0
173.80	57264.0
174.90	4029.0
175.80	55032.0
176.80	3672.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	484.0
36.90	3012.0
37.90	2629.0
38.90	1144.0
39.90	267.0
43.90	840.0
44.80	514.0
46.90	611.0
47.80	312.0
48.90	2624.0
49.90	12277.0
51.00	4068.0
51.90	160.0
55.00	155.0
55.90	1042.0
56.90	1994.0
58.00	119.0
59.90	686.0
60.90	3367.0
62.00	3254.0
63.00	2569.0
64.00	332.0
64.80	107.0
67.00	187.0
67.90	7255.0
68.90	7855.0
69.90	611.0
71.90	403.0
73.00	3229.0
73.90	12454.0
75.00	36800.0
75.90	3210.0
76.90	419.0
77.80	256.0
78.80	2502.0
79.80	774.0
80.90	2625.0
81.80	642.0
86.90	2793.0
87.90	2799.0
90.80	370.0
91.90	2169.0
92.90	3327.0
93.90	8955.0
94.90	70016.0
95.90	4742.0
96.90	137.0
103.80	386.0
104.80	136.0
105.80	370.0
112.70	109.0
115.90	215.0
116.90	443.0
117.70	256.0
118.80	267.0
127.80	318.0
128.70	130.0
129.70	242.0
130.90	148.0
134.90	101.0
136.60	110.0
140.70	773.0
142.80	795.0
147.80	114.0
154.70	178.0
156.80	130.0
158.70	158.0
171.80	279.0
172.90	438.0
173.80	56272.0
174.80	4000.0
175.80	53072.0
176.80	3442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015