

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
 Data File : VU051545.D
 Acq On : 27 Oct 2022 17:33
 Operator : JC/MD
 Sample : N5270-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	90	rBV	111124	137920	13.91%	1.688%
2	1.909	169	177	200	rVB	104508	143120	14.43%	1.752%
3	2.565	369	381	393	rBV	163628	264485	26.67%	3.238%
4	2.629	394	401	418	rVB2	12661	24607	2.48%	0.301%
5	2.781	432	448	463	rBV2	11422	30591	3.09%	0.374%
6	3.186	559	574	595	rBV	4556	11066	1.12%	0.135%
7	3.883	765	791	812	rVB	11503	49618	5.00%	0.607%
8	4.623	1005	1021	1052	rBV	173861	442661	44.64%	5.419%
9	5.067	1139	1159	1188	rBV3	214940	656142	66.17%	8.032%
10	5.723	1341	1363	1389	rBV2	351218	935036	94.30%	11.446%
11	6.247	1509	1526	1547	rBV	329496	630559	63.59%	7.719%
12	6.690	1650	1664	1689	rBV	227030	448529	45.23%	5.491%
13	7.565	1923	1936	1954	rBV	90261	162381	16.38%	1.988%
14	7.896	2025	2039	2054	rBV	365838	639126	64.45%	7.824%
15	7.970	2054	2062	2075	rVB	29983	53647	5.41%	0.657%
16	8.179	2116	2127	2140	rBV	54581	92085	9.29%	1.127%
17	8.472	2207	2218	2230	rBV2	6375	11413	1.15%	0.140%
18	8.632	2256	2268	2304	rBV	528003	991588	100.00%	12.139%
19	8.787	2308	2316	2331	rVB9	12737	24327	2.45%	0.298%
20	9.417	2499	2512	2536	rBV	479620	804272	81.11%	9.846%
21	9.693	2588	2598	2611	rBV2	16156	28429	2.87%	0.348%
22	10.102	2716	2725	2739	rBV6	6734	13272	1.34%	0.162%
23	10.754	2913	2928	2944	rBV	187447	301018	30.36%	3.685%
24	10.893	2961	2971	2983	rBV2	13180	20922	2.11%	0.256%
25	11.809	3244	3256	3277	rBV	404491	661962	66.76%	8.104%
26	12.063	3325	3335	3350	rBV5	9109	18638	1.88%	0.228%
27	12.192	3362	3375	3397	rBV	328895	550594	55.53%	6.740%
28	12.886	3583	3591	3601	rBV7	12672	20816	2.10%	0.255%




Sum of corrected areas: 8168824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051545.D
Acq On : 27 Oct 2022 17:33
Operator : JC/MD
Sample : N5270-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAEO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

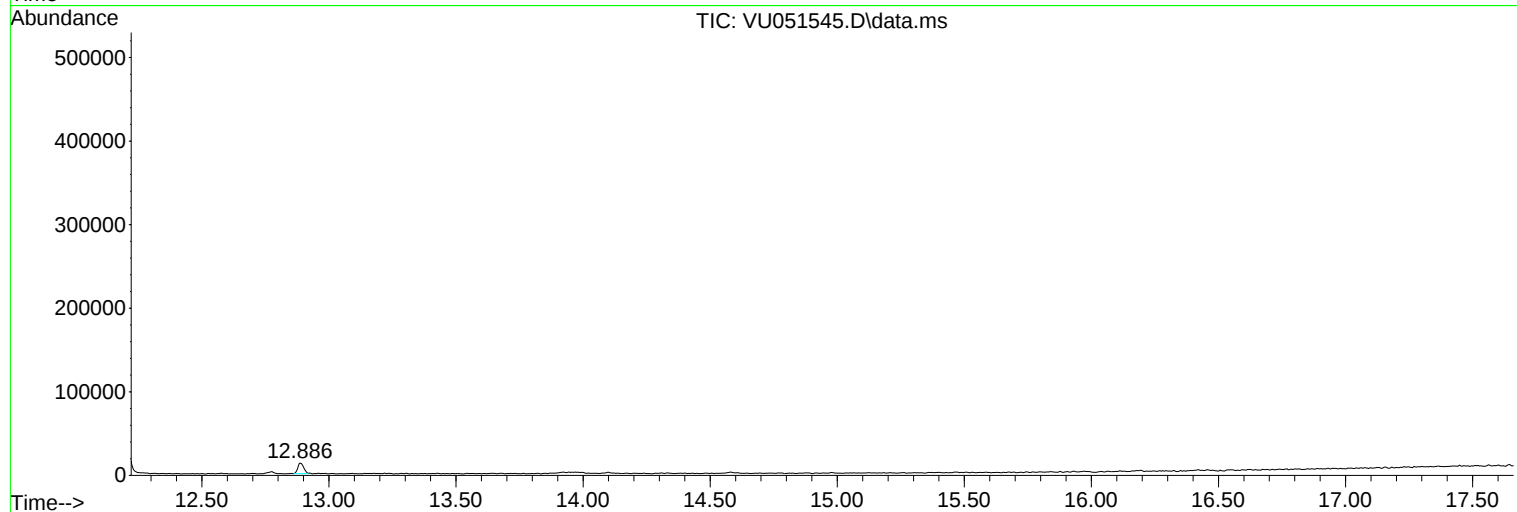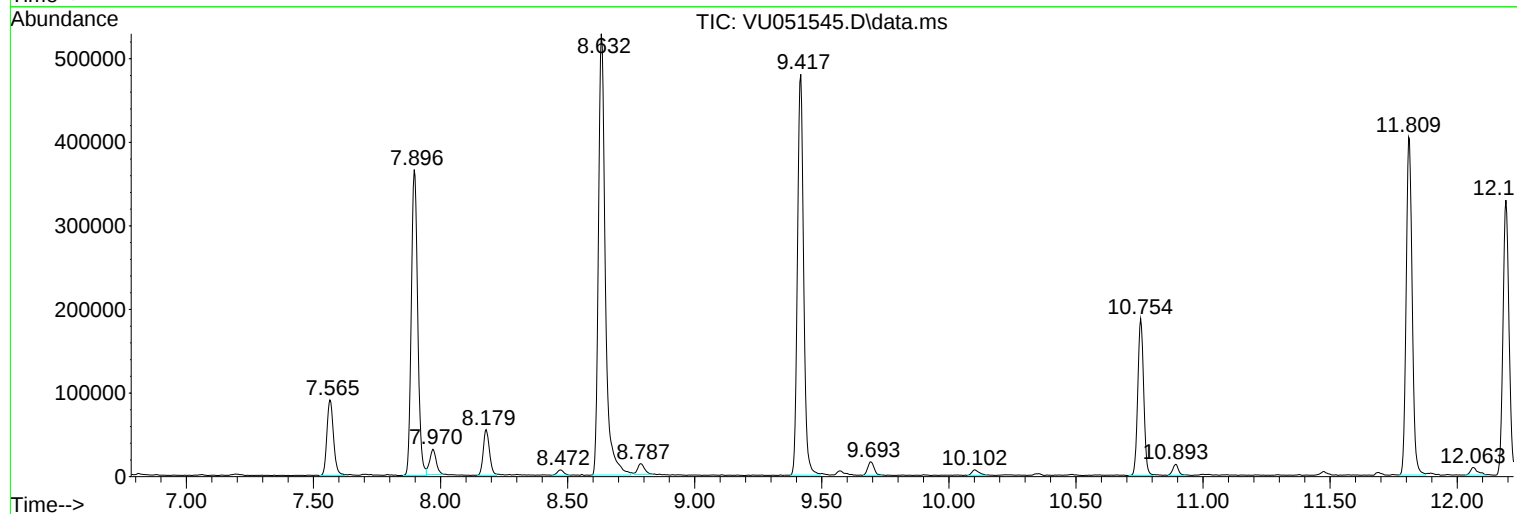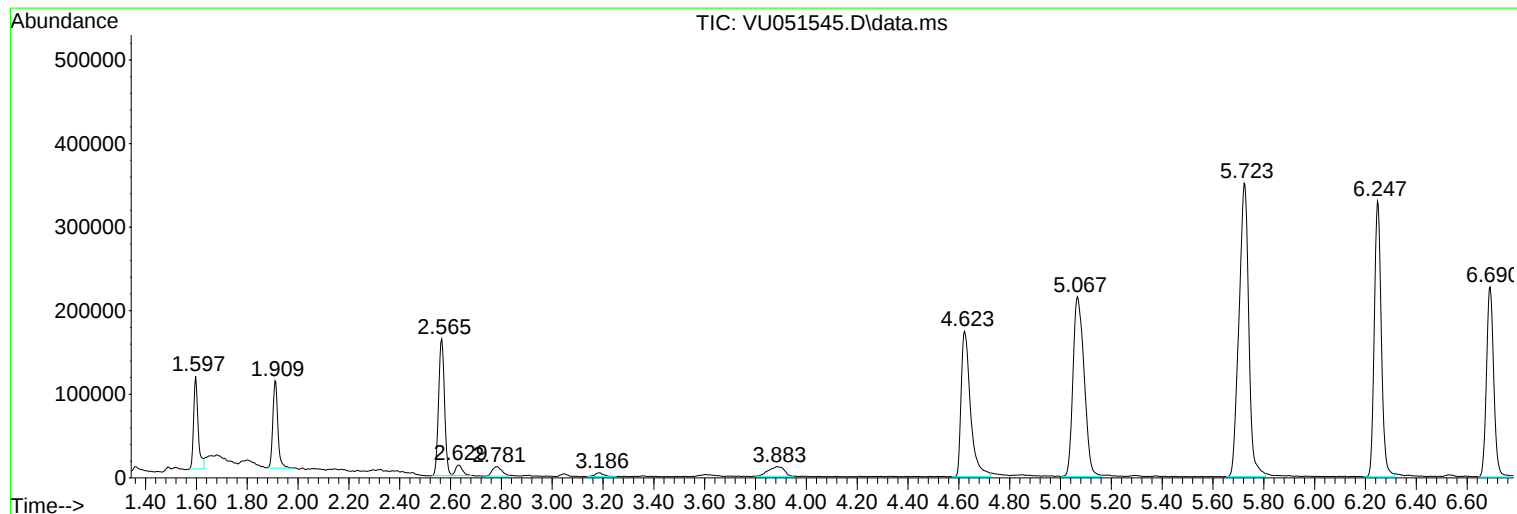

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051545.D
Acq On : 27 Oct 2022 17:33
Operator : JC/MD
Sample : N5270-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051545.D
Acq On : 27 Oct 2022 17:33
Operator : JC/MD
Sample : N5270-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
