

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
 Data File : VU051551.D
 Acq On : 27 Oct 2022 20:04
 Operator : JC/MD
 Sample : N5300-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	107259	127684	12.45%	1.622%
2	1.912	170	178	194	rBV	102451	136444	13.30%	1.733%
3	2.565	369	381	396	rVB	161209	258645	25.22%	3.286%
4	2.652	396	408	429	rBV	10138	26927	2.63%	0.342%
5	3.877	757	789	810	rVB	13621	65058	6.34%	0.826%
6	4.633	1009	1024	1063	rBV	156299	467912	45.62%	5.944%
7	5.063	1142	1158	1187	rBV3	203458	606834	59.16%	7.709%
8	5.723	1343	1363	1389	rBV2	341899	911213	88.83%	11.576%
9	6.247	1513	1526	1547	rBV	297617	579577	56.50%	7.363%
10	6.690	1650	1664	1692	rBV	225845	443885	43.27%	5.639%
11	7.565	1924	1936	1954	rBV	85272	152770	14.89%	1.941%
12	7.896	2022	2039	2054	rBV	351510	609335	59.40%	7.741%
13	7.970	2054	2062	2075	rVB	29718	53458	5.21%	0.679%
14	8.179	2116	2127	2146	rBV2	53243	93147	9.08%	1.183%
15	8.472	2207	2218	2228	rBV2	5841	10841	1.06%	0.138%
16	8.632	2253	2268	2308	rBV	518429	1025755	100.00%	13.031%
17	8.790	2308	2317	2329	rVB4	13753	23632	2.30%	0.300%
18	9.417	2499	2512	2536	rBV	446036	748801	73.00%	9.512%
19	9.690	2587	2597	2614	rVB3	15740	26523	2.59%	0.337%
20	10.102	2715	2725	2738	rVB3	6060	11585	1.13%	0.147%
21	10.755	2915	2928	2949	rBV	187930	304359	29.67%	3.866%
22	10.890	2962	2970	2983	rVB2	11362	18912	1.84%	0.240%
23	11.809	3241	3256	3279	rBV	367341	597963	58.29%	7.596%
24	12.063	3325	3335	3352	rBV3	11845	22244	2.17%	0.283%
25	12.192	3360	3375	3398	rBV	320767	527827	51.46%	6.705%
26	12.890	3583	3592	3605	rVB6	12833	20434	1.99%	0.260%




Sum of corrected areas: 7871765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051551.D
Acq On : 27 Oct 2022 20:04
Operator : JC/MD
Sample : N5300-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

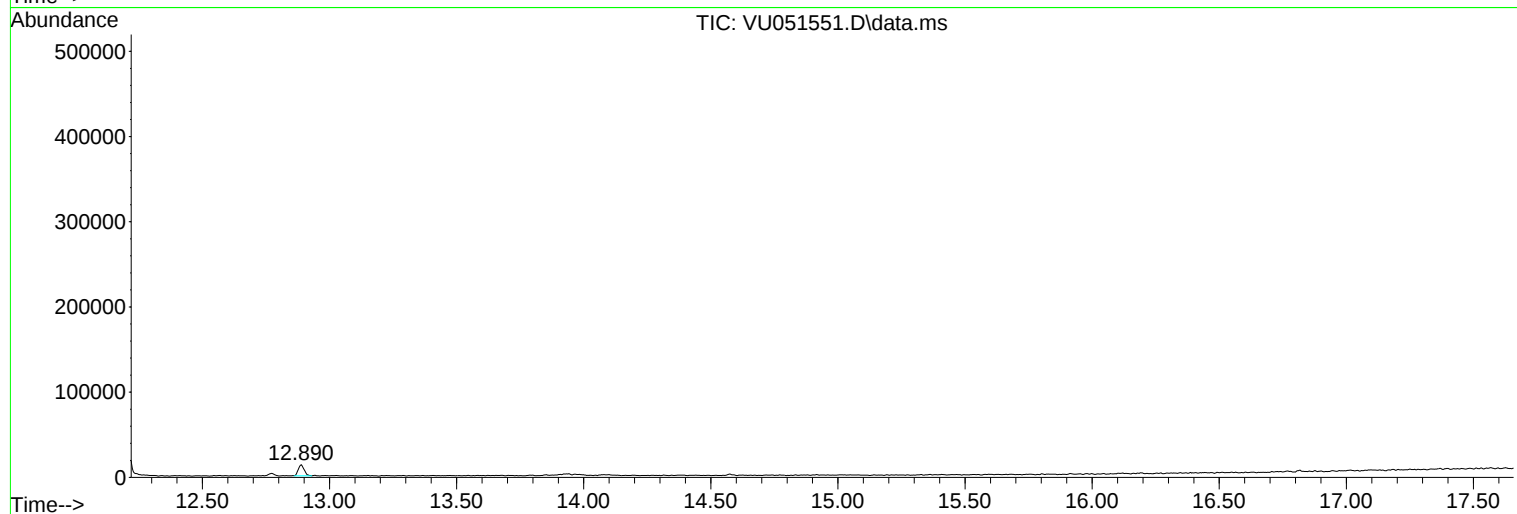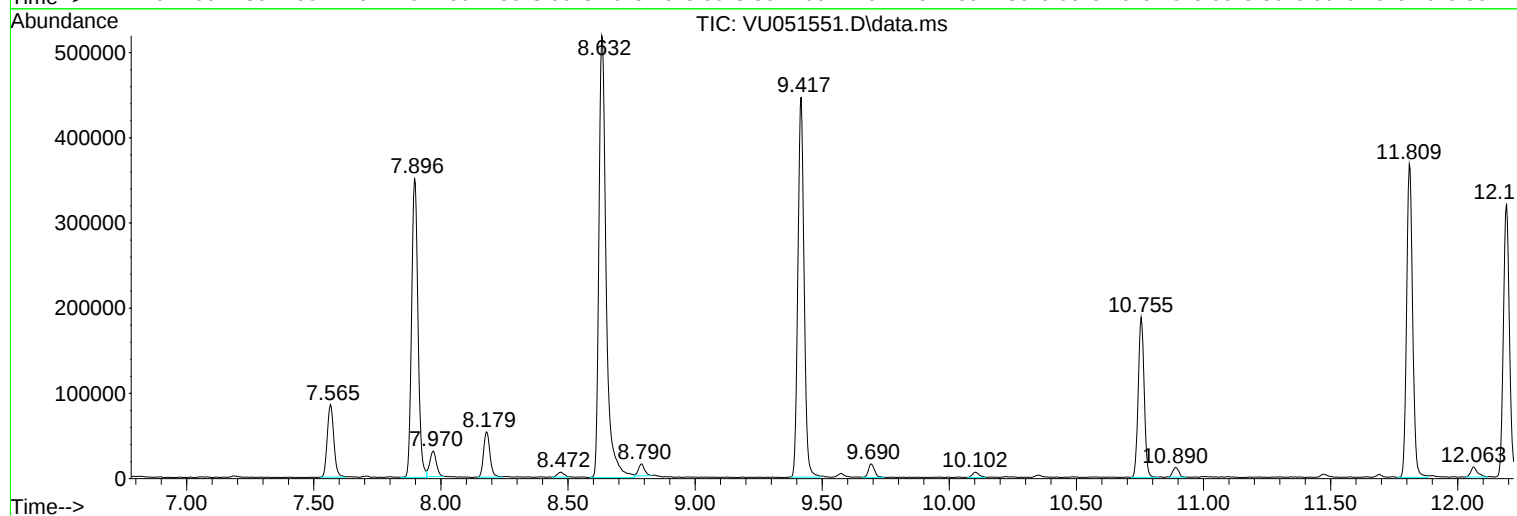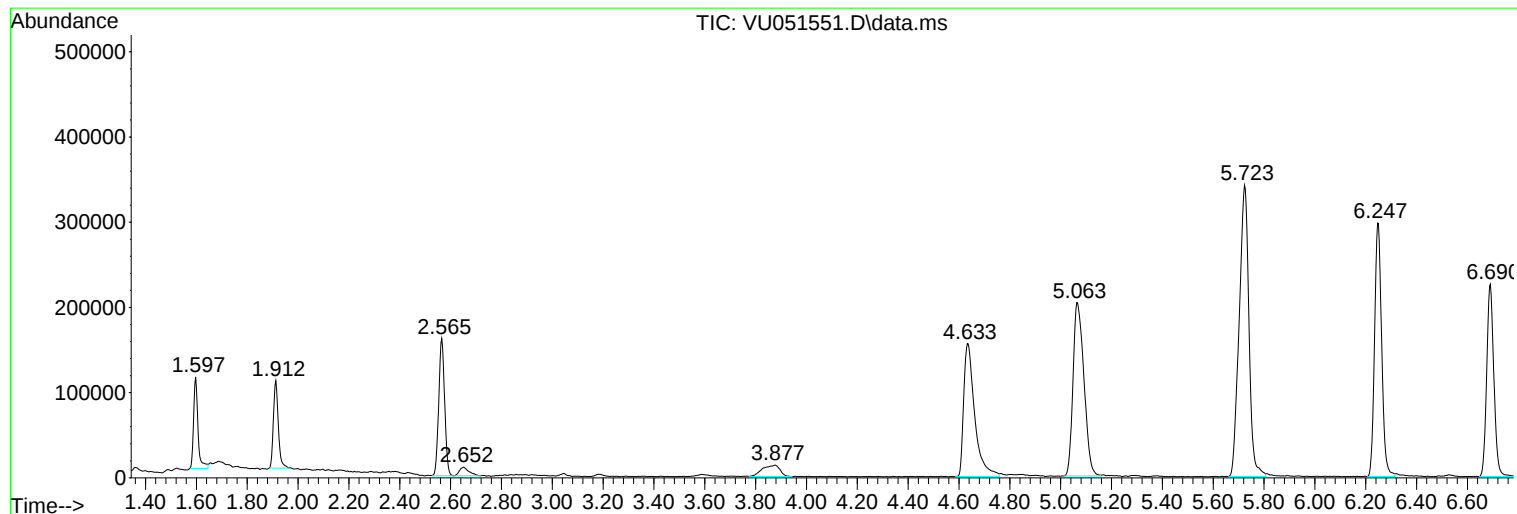

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051551.D
Acq On : 27 Oct 2022 20:04
Operator : JC/MD
Sample : N5300-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
Data File : VU051551.D
Acq On : 27 Oct 2022 20:04
Operator : JC/MD
Sample : N5300-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc