


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102722\
 Data File : VU051537.D
 Acq On : 27 Oct 2022 13:35
 Operator : JC/MD
 Sample : BFB158
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB158

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 28 00:08:00 2022

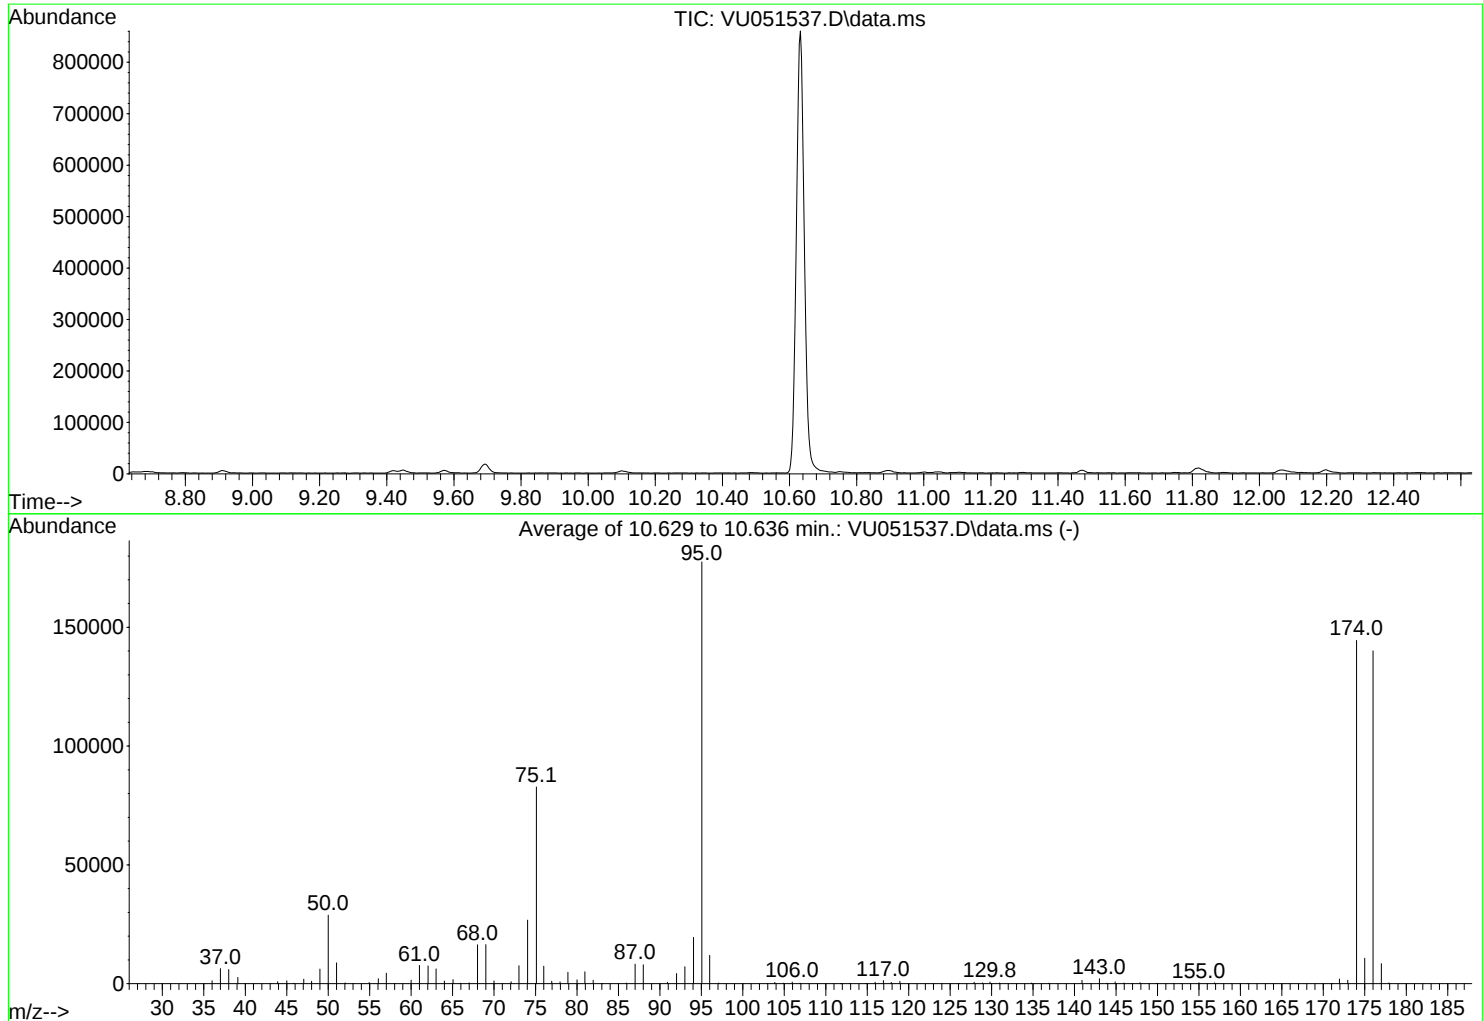

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	28829	PASS
75	95	30	80	46.6	82811	PASS
95	95	100	100	100.0	177557	PASS
96	95	5	9	6.7	11925	PASS
173	174	0.00	2	1.0	1444	PASS
174	95	50	120	81.4	144491	PASS
175	174	5	9	7.4	10722	PASS
176	174	95	101	97.0	140117	PASS
177	176	5	9	6.0	8448	PASS

m/z	Abundance
40.00	1048.0
43.90	725.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

m/z	Abundance
36.00	1202.0
37.00	6606.0
38.00	6103.0
39.10	2812.0
39.90	1031.0
43.00	159.0
44.00	1591.0
45.00	1304.0
45.80	170.0
47.10	2214.0
48.00	1033.0
49.00	6277.0
50.00	29952.0
51.00	8970.0
52.00	353.0
53.00	107.0
54.90	528.0
56.00	2006.0
57.00	4560.0
58.00	170.0
60.00	1526.0
61.00	8201.0
62.00	7677.0
63.00	6380.0
64.00	1150.0
65.10	1857.0
65.90	243.0
67.00	454.0
68.00	16169.0
69.00	16568.0
70.00	1141.0
71.00	106.0
72.10	757.0
73.00	7661.0
74.10	26696.0
75.10	83952.0
76.00	7532.0
76.90	1012.0
77.90	689.0
78.90	4783.0
80.00	1804.0
80.90	5084.0
82.00	1450.0
83.00	102.0
85.90	329.0
87.00	7974.0
88.00	7837.0
90.90	553.0
92.00	4534.0
93.00	7200.0
94.10	19376.0
95.10	178368.0
96.00	12148.0
97.10	314.0
102.90	123.0
103.80	565.0
104.90	214.0
105.90	652.0
106.90	185.0
114.80	163.0
115.90	671.0
117.00	1327.0
117.90	590.0
119.00	1014.0
124.00	156.0
126.00	103.0
127.90	592.0
128.90	334.0
129.80	661.0
130.90	299.0
134.80	280.0
136.90	205.0
140.90	1437.0
141.90	117.0
143.00	2134.0
143.90	173.0
144.90	785.0
146.00	259.0
147.00	131.0
147.90	441.0
148.90	124.0
149.90	119.0
151.90	156.0
152.80	176.0
155.00	373.0
156.90	359.0
160.90	115.0
170.90	237.0
172.00	1971.0
172.90	1456.0
174.00	141184.0
175.00	10938.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

176.00

177.00

177.90

137408.0

8389.0

312.0

Instrument :

MSVOA_U

ClientSampleId :

BFB158

m/z	Abundance
36.00	1227.0
37.00	6525.0
38.00	6091.0
39.10	2737.0
39.90	909.0
43.00	145.0
43.90	1562.0
45.00	1279.0
45.90	191.0
47.00	1896.0
48.00	1076.0
49.00	6245.0
50.00	29712.0
51.00	9036.0
52.00	350.0
53.00	136.0
54.90	500.0
56.00	2135.0
57.00	4447.0
58.00	164.0
60.00	1496.0
61.00	7807.0
62.10	7617.0
63.00	6408.0
64.00	1172.0
65.10	1730.0
65.90	239.0
67.00	347.0
68.00	16816.0
69.00	16976.0
70.00	1184.0
71.00	107.0
72.10	847.0
73.00	7769.0
74.00	27464.0
75.10	85424.0
76.00	7516.0
77.00	1088.0
78.00	785.0
78.90	4878.0
80.00	1687.0
81.00	5115.0
81.90	1521.0
85.90	290.0
87.00	8535.0
88.00	8271.0
90.90	602.0
92.00	4348.0
93.00	7397.0
94.10	20152.0
95.10	182720.0
96.00	12285.0
97.10	316.0
103.80	574.0
104.90	213.0
106.00	710.0
106.90	217.0
111.80	103.0
112.90	170.0
114.80	138.0
115.90	610.0
117.00	1350.0
117.90	625.0
119.00	1066.0
124.00	172.0
127.90	662.0
128.90	391.0
129.80	773.0
131.00	303.0
134.80	311.0
136.90	205.0
140.00	120.0
140.90	1484.0
143.00	2155.0
143.90	235.0
144.90	788.0
145.90	261.0
147.00	168.0
147.90	432.0
148.90	103.0
149.90	179.0
151.90	117.0
152.80	111.0
155.00	404.0
156.90	370.0
158.90	106.0
160.90	109.0
171.10	231.0
172.00	1989.0
173.00	1506.0
174.00	149056.0
175.00	11054.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

176.00144768.0

177.008715.0

177.90333.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158

m/z	Abundance
36.00	1128.0
37.00	5911.0
38.00	5546.0
39.10	2401.0
39.90	867.0
43.10	154.0
43.90	1554.0
45.00	1086.0
45.90	240.0
47.10	1565.0
48.00	918.0
49.00	5803.0
50.00	26824.0
51.00	8219.0
52.10	352.0
53.00	150.0
55.00	460.0
56.10	2065.0
57.00	4103.0
58.00	173.0
60.00	1431.0
61.00	6935.0
62.10	7060.0
63.00	5926.0
64.00	946.0
65.00	1433.0
66.00	203.0
67.00	269.0
68.00	16184.0
69.00	15823.0
70.00	1143.0
71.00	103.0
72.00	924.0
73.00	7183.0
74.00	25976.0
75.10	79056.0
76.00	6905.0
77.00	993.0
78.00	784.0
78.90	4698.0
80.00	1399.0
80.90	4733.0
81.90	1366.0
86.00	255.0
87.00	8168.0
88.00	7783.0
90.90	583.0
92.00	3941.0
93.00	6833.0
94.00	18880.0
95.00	171584.0
96.00	11342.0
97.10	279.0
103.90	555.0
104.90	187.0
106.00	717.0
106.90	195.0
112.90	167.0
116.00	524.0
116.90	1268.0
117.90	495.0
118.90	1056.0
124.00	122.0
127.90	682.0
128.90	363.0
129.80	695.0
130.90	254.0
134.80	279.0
136.90	188.0
140.00	139.0
140.90	1362.0
141.90	106.0
143.00	2021.0
143.90	266.0
144.90	699.0
145.90	244.0
147.00	174.0
147.90	419.0
149.90	192.0
152.00	126.0
155.00	384.0
156.90	317.0
158.90	132.0
160.90	119.0
171.10	227.0
171.90	1889.0
173.00	1370.0
174.00	143232.0
175.00	10173.0
176.00	138176.0
177.00	8241.0
177.90	364.0

Instrument :
MSVOA_U
ClientSampleId :
BFB158