

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
 Data File : VU061263.D
 Acq On : 28 Oct 2024 12:48
 Operator : MD/SY
 Sample : VIBLK151
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK151

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU061263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	107	rBV	63249	74904	12.00%	1.427%
2	1.911	184	193	206	rBV	54120	73902	11.84%	1.408%
3	2.560	380	395	413	rVB	106485	176717	28.31%	3.367%
4	3.177	573	587	603	rBV2	13083	28995	4.65%	0.552%
5	4.631	1023	1039	1089	rBV2	87306	263243	42.17%	5.015%
6	5.055	1156	1171	1196	rBV	104850	236206	37.84%	4.500%
7	5.718	1355	1377	1410	rBV2	206453	548511	87.87%	10.450%
8	6.242	1528	1540	1574	rBV	257148	497869	79.76%	9.485%
9	6.682	1664	1677	1703	rBV	126515	253325	40.58%	4.826%
10	7.560	1938	1950	1974	rBV	68086	126842	20.32%	2.416%
11	7.891	2037	2053	2073	rBV	248634	451286	72.30%	8.598%
12	8.177	2130	2142	2162	rBV	38181	70273	11.26%	1.339%
13	8.631	2267	2283	2324	rBV2	251854	555133	88.94%	10.576%
14	9.412	2514	2526	2565	rBV	354635	624200	100.00%	11.892%
15	9.569	2565	2575	2588	rVB	6839	10876	1.74%	0.207%
16	9.692	2605	2613	2630	rBV3	6621	10916	1.75%	0.208%
17	10.750	2931	2942	2964	rBV	94670	156761	25.11%	2.986%
18	11.807	3258	3271	3298	rBV	334726	582140	93.26%	11.090%
19	12.187	3375	3389	3411	rBV	223227	408377	65.42%	7.780%
20	13.839	3890	3903	3926	rBV2	53072	98546	15.79%	1.877%




Sum of corrected areas: 5249022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061263.D
Acq On : 28 Oct 2024 12:48
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

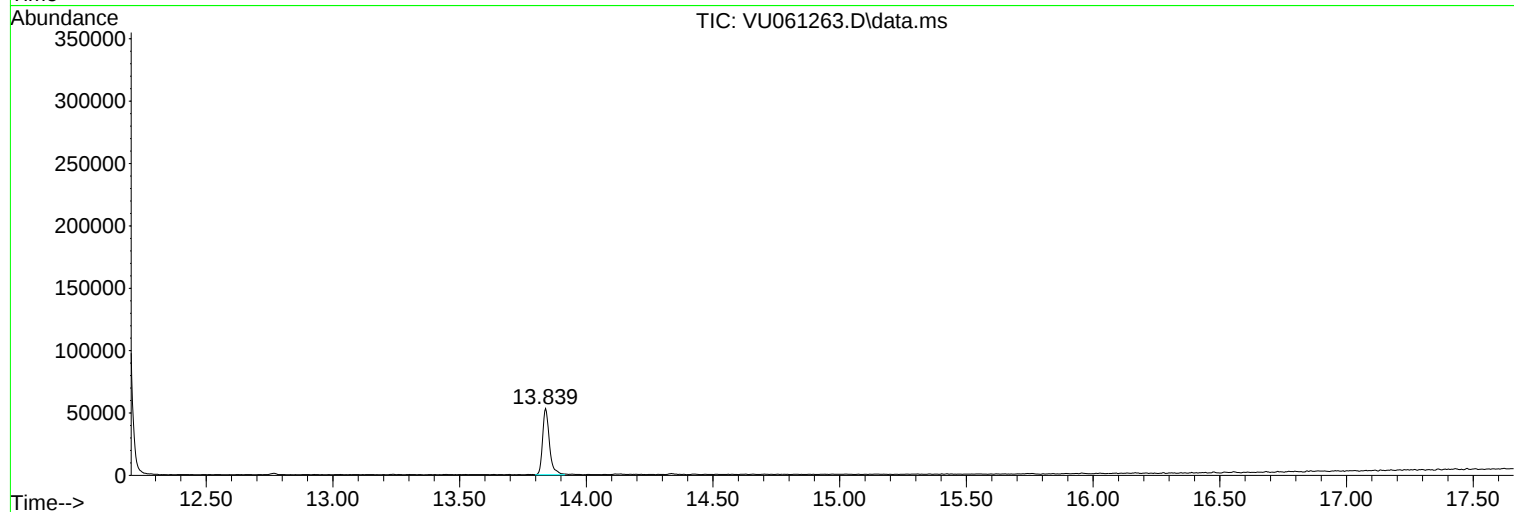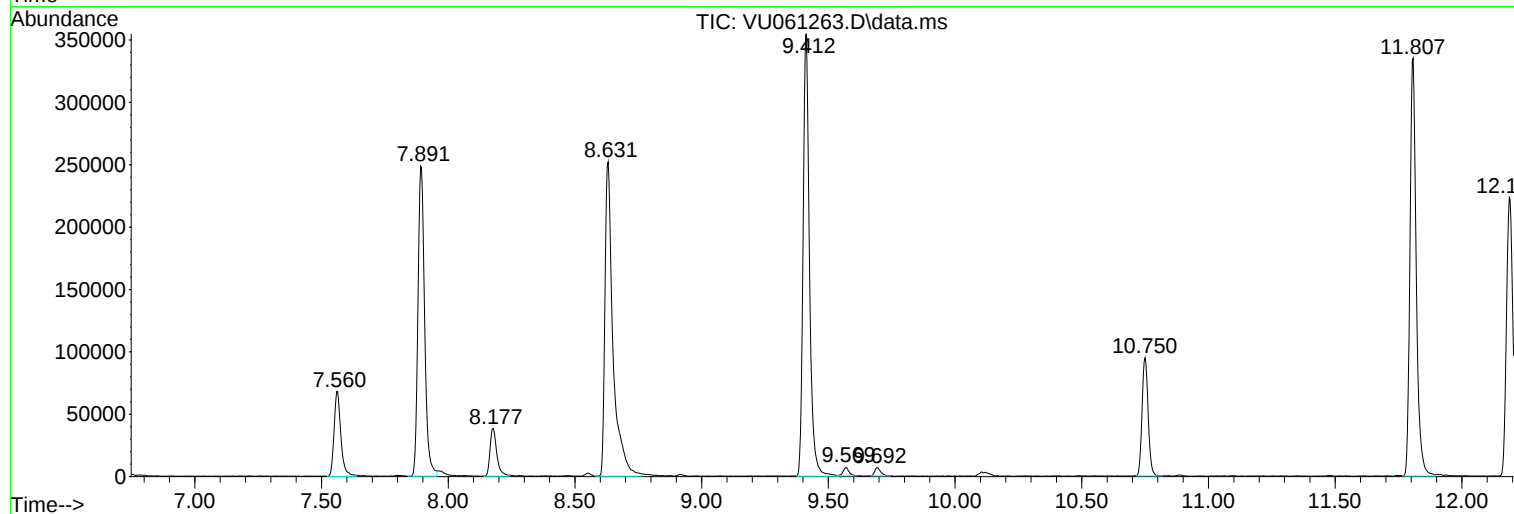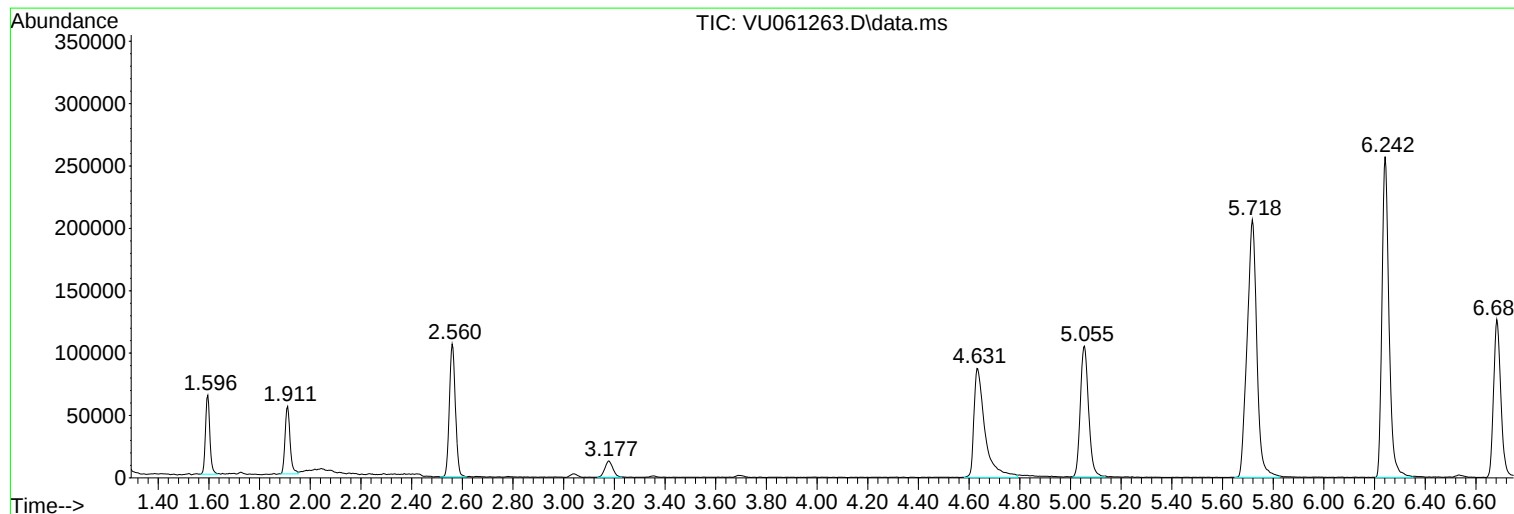

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061263.D
Acq On : 28 Oct 2024 12:48
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061263.D
Acq On : 28 Oct 2024 12:48
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc