

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
 Data File : VU061265.D
 Acq On : 28 Oct 2024 14:27
 Operator : MD/SY
 Sample : P4536-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU061265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	110	rBV	64854	74906	13.02%	1.532%
2	1.911	181	193	212	rBV	62487	90653	15.76%	1.854%
3	2.560	383	395	412	rBV	110513	181001	31.47%	3.701%
4	3.042	532	545	557	rBV	5587	10474	1.82%	0.214%
5	4.628	1028	1038	1081	rBV	76606	214644	37.32%	4.389%
6	5.055	1156	1171	1193	rBV	110958	247702	43.07%	5.065%
7	5.717	1356	1377	1418	rBV2	212153	561977	97.72%	11.490%
8	6.242	1528	1540	1568	rBV	212428	415519	72.25%	8.496%
9	6.682	1664	1677	1705	rBV	133536	266047	46.26%	5.440%
10	7.560	1939	1950	1975	rBV	68448	127955	22.25%	2.616%
11	7.891	2042	2053	2074	rBV	253827	463009	80.51%	9.467%
12	8.177	2131	2142	2165	rBV2	39468	72426	12.59%	1.481%
13	8.631	2271	2283	2314	rBV2	280483	575099	100.00%	11.759%
14	9.412	2514	2526	2547	rBV	284500	508676	88.45%	10.401%
15	9.573	2567	2576	2586	rVB2	3458	5934	1.03%	0.121%
16	9.698	2602	2615	2632	rVB3	3392	6891	1.20%	0.141%
17	10.749	2931	2942	2966	rVB	99161	163804	28.48%	3.349%
18	11.807	3259	3271	3303	rBV	272174	466633	81.14%	9.541%
19	12.187	3377	3389	3412	rBV	224118	396149	68.88%	8.100%
20	13.843	3891	3904	3924	rBV2	21032	41352	7.19%	0.845%




Sum of corrected areas: 4890851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061265.D
Acq On : 28 Oct 2024 14:27
Operator : MD/SY
Sample : P4536-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

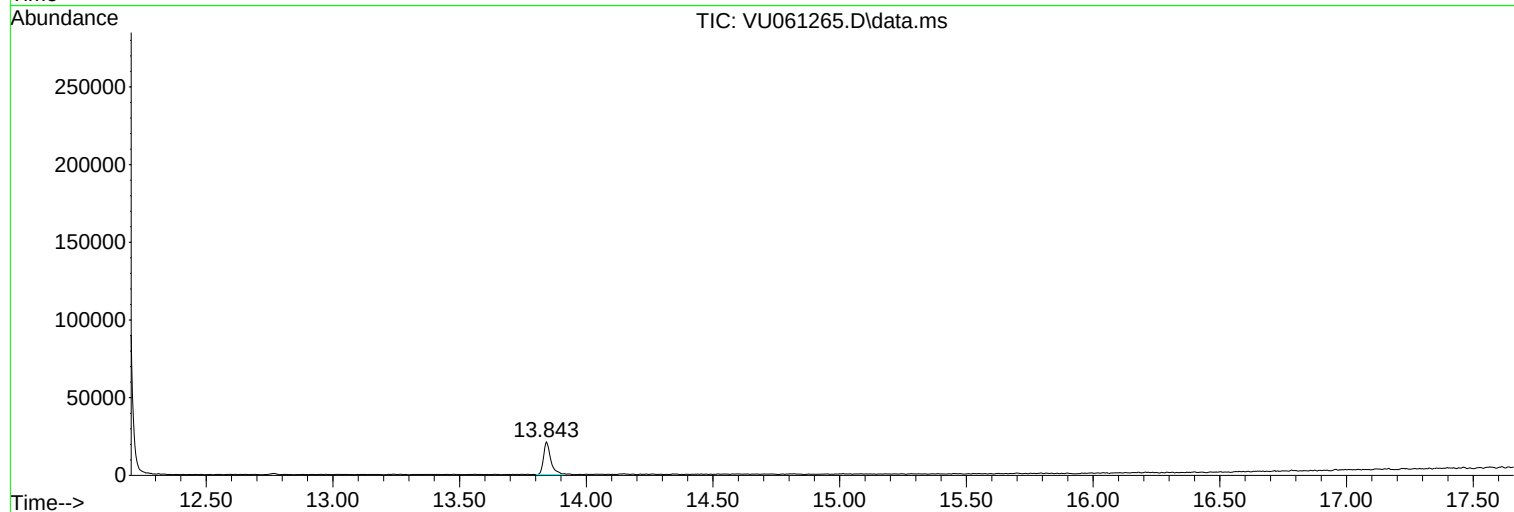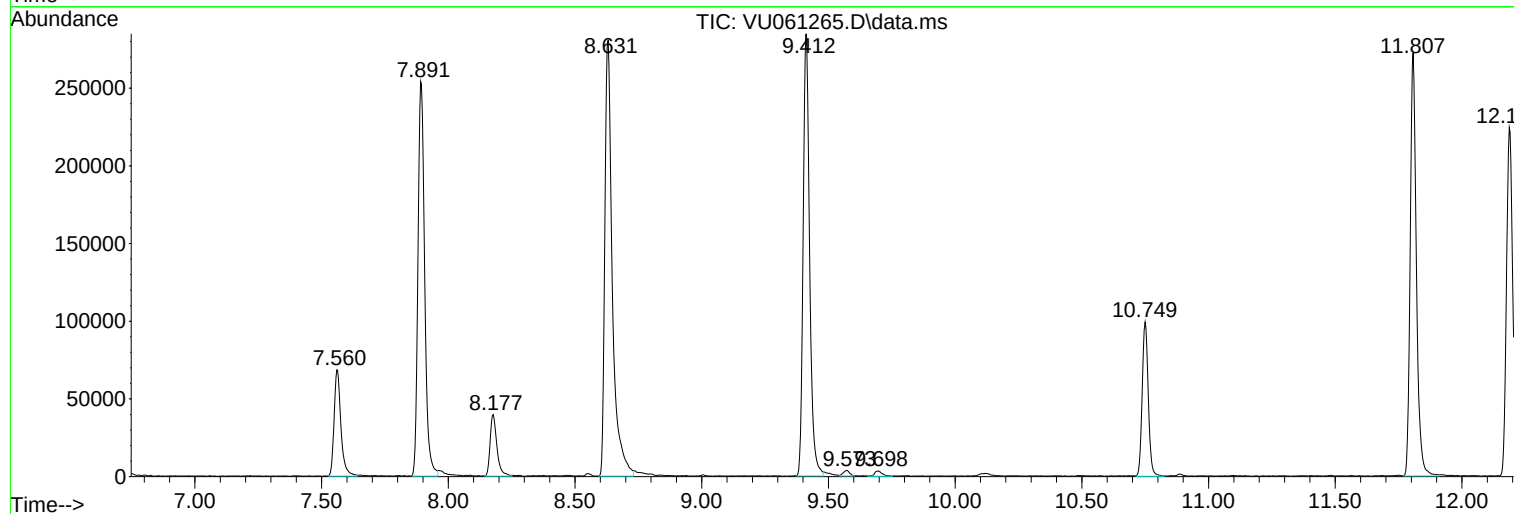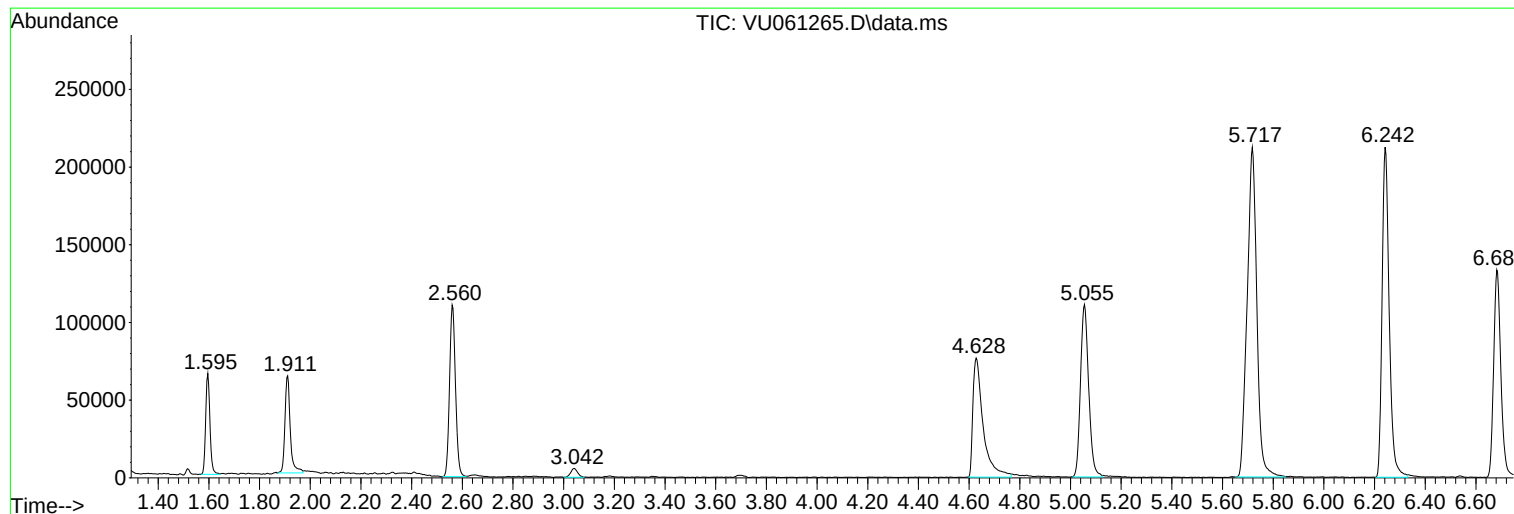

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061265.D
Acq On : 28 Oct 2024 14:27
Operator : MD/SY
Sample : P4536-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061265.D
Acq On : 28 Oct 2024 14:27
Operator : MD/SY
Sample : P4536-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc