


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102824\
Data File : VU061259.D
Acq On : 28 Oct 2024 08:51
Operator : MD/SY
Sample : BFB016
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB016

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 29 04:45:10 2024

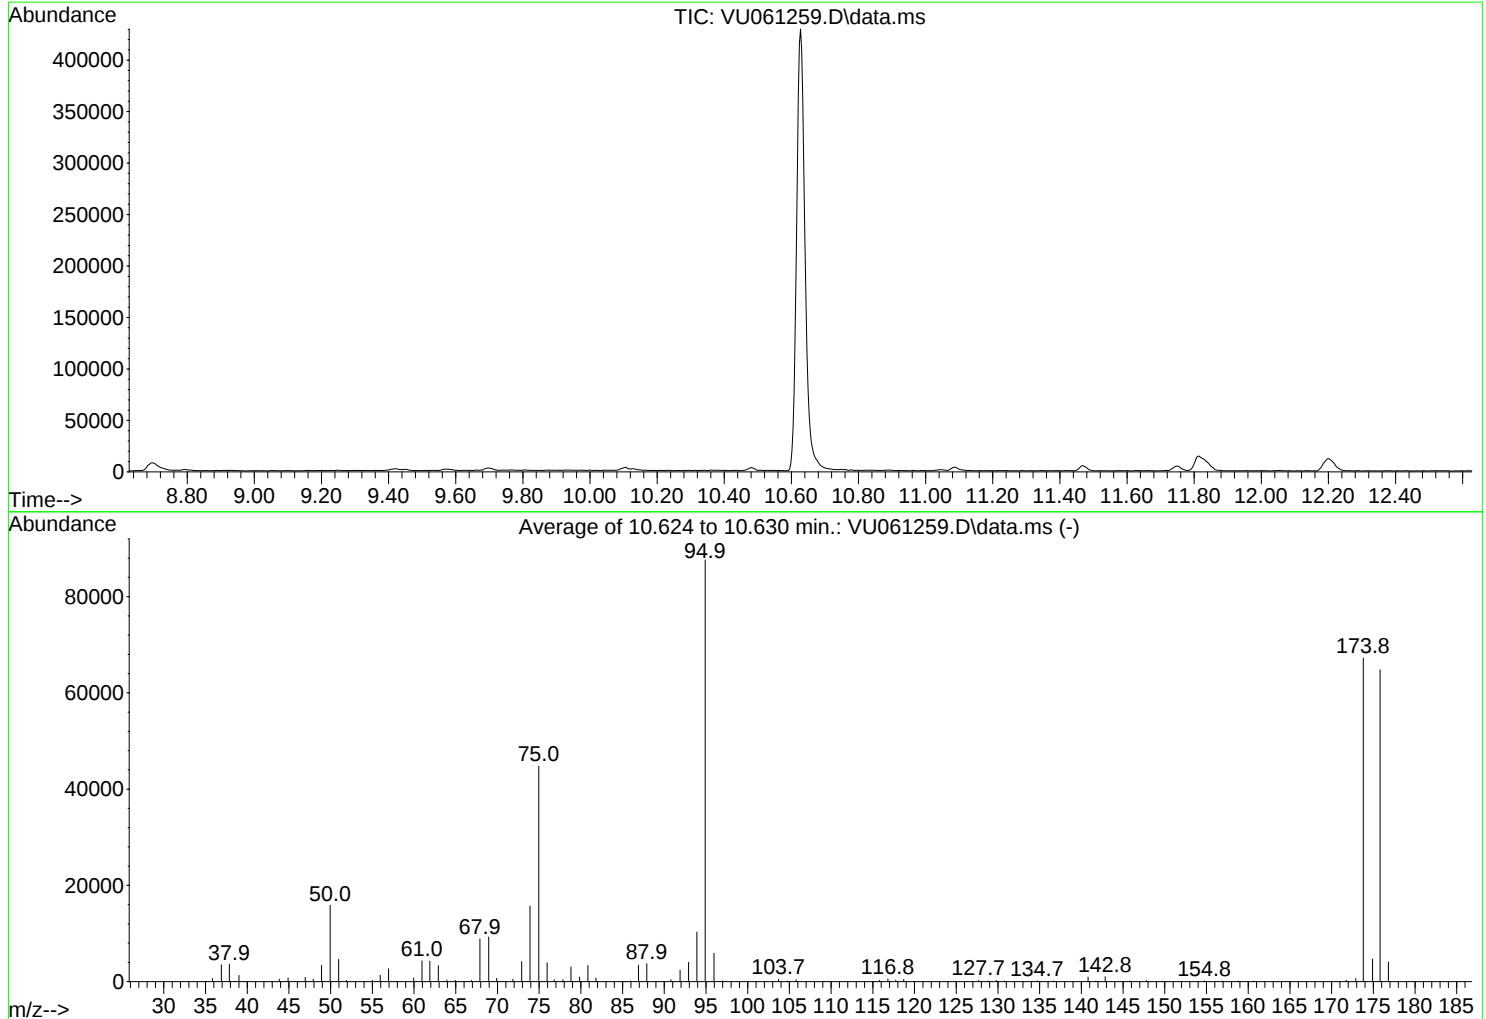

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	15859	PASS
75	95	30	80	51.1	44755	PASS
95	95	100	100	100.0	87640	PASS
96	95	5	9	6.7	5874	PASS
173	174	0.00	2	0.9	632	PASS
174	95	50	120	76.7	67208	PASS
175	174	5	9	7.0	4734	PASS
176	174	95	101	96.4	64800	PASS
177	176	5	9	6.3	4068	PASS

m/z	Abundance
35.90	493.0
37.80	199.0
39.70	172.0
43.80	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1157.0
36.90	3583.0
37.90	3821.0
39.00	1296.0
39.80	191.0
42.90	105.0
43.90	873.0
44.90	791.0
47.00	858.0
47.90	479.0
48.90	3447.0
50.00	15733.0
50.90	4643.0
51.90	240.0
55.00	261.0
55.90	1324.0
56.90	2660.0
59.90	807.0
60.90	4403.0
61.90	4279.0
62.90	3512.0
64.00	306.0
64.90	292.0
66.90	253.0
67.90	8863.0
68.90	9360.0
69.90	696.0
71.90	477.0
72.90	4081.0
73.90	15770.0
75.00	45192.0
76.00	3939.0
76.80	421.0
77.80	349.0
78.80	3077.0
79.80	946.0
80.80	3303.0
81.80	727.0
86.00	150.0
86.90	3279.0
87.90	3769.0
90.80	370.0
91.90	2410.0
92.90	3910.0
93.90	10488.0
94.90	87384.0
96.00	6071.0
97.00	210.0
103.70	536.0
104.80	148.0
105.80	452.0
115.80	303.0
116.80	553.0
117.70	312.0
118.70	435.0
127.70	301.0
128.80	174.0
129.80	278.0
130.70	134.0
134.70	117.0
136.70	156.0
140.80	971.0
141.90	130.0
142.90	982.0
145.80	111.0
147.80	239.0
149.70	148.0
154.70	173.0
156.90	122.0
158.80	174.0
160.70	101.0
171.70	290.0
172.90	650.0
173.80	66232.0
174.90	4650.0
175.80	62912.0
176.80	4146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1174.0
36.90	3587.0
37.90	3862.0
39.00	1335.0
39.80	179.0
43.90	828.0
44.90	785.0
47.00	944.0
47.90	490.0
48.90	3461.0
49.90	16290.0
50.90	4732.0
51.90	233.0
55.00	267.0
55.90	1382.0
56.90	2695.0
60.00	778.0
61.00	4500.0
61.90	4399.0
62.90	3396.0
63.90	337.0
65.00	274.0
66.90	287.0
67.90	9053.0
69.00	9471.0
69.90	741.0
71.80	524.0
72.90	4313.0
73.90	16195.0
74.90	46048.0
75.90	4102.0
76.80	398.0
77.80	399.0
78.80	3139.0
79.90	1001.0
80.80	3447.0
81.80	810.0
86.00	155.0
86.90	3572.0
87.90	3878.0
90.80	393.0
91.90	2465.0
92.90	4091.0
93.90	10558.0
94.90	90056.0
95.90	6052.0
97.00	173.0
103.70	490.0
104.70	146.0
105.80	400.0
115.80	274.0
116.80	604.0
117.80	317.0
118.70	473.0
127.70	313.0
128.80	136.0
129.80	278.0
130.80	114.0
134.70	162.0
136.70	171.0
140.80	991.0
141.70	121.0
142.80	1067.0
145.80	154.0
147.80	259.0
149.70	132.0
154.70	175.0
156.90	155.0
158.80	151.0
160.70	115.0
171.70	308.0
172.90	648.0
173.80	68936.0
174.90	4888.0
175.80	66856.0
176.80	4106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	1095.0
36.90	3404.0
37.90	3664.0
39.00	1240.0
39.80	139.0
43.90	685.0
44.90	698.0
46.90	883.0
47.90	485.0
48.90	3227.0
49.90	15553.0
51.00	4485.0
51.90	212.0
55.00	273.0
56.00	1424.0
57.00	2589.0
57.90	105.0
60.00	747.0
61.00	4109.0
61.90	4131.0
62.90	3058.0
63.90	366.0
65.00	235.0
66.90	290.0
67.90	8696.0
69.00	8975.0
69.90	699.0
71.80	484.0
72.90	4147.0
73.90	15161.0
74.90	43024.0
75.90	3773.0
76.80	362.0
77.90	408.0
78.80	2984.0
79.90	904.0
80.90	3311.0
81.80	801.0
85.90	123.0
86.90	3447.0
87.90	3560.0
90.80	391.0
91.90	2346.0
92.90	3978.0
93.90	9896.0
94.90	85480.0
95.90	5499.0
97.00	137.0
103.70	401.0
104.80	126.0
105.80	350.0
115.80	263.0
116.80	556.0
117.80	337.0
118.70	476.0
127.70	313.0
128.80	108.0
129.80	257.0
130.80	112.0
134.70	181.0
136.70	176.0
140.80	938.0
141.60	127.0
142.80	1047.0
145.80	171.0
147.80	229.0
154.80	170.0
156.90	145.0
158.80	112.0
160.70	100.0
171.80	307.0
172.90	599.0
173.80	66456.0
174.90	4663.0
175.80	64632.0
176.80	3953.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016