

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061282.D
 Acq On : 29 Oct 2024 14:08
 Operator : MD/SY
 Sample : P4436-11
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 29 22:34:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 29 22:33:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	178005	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	161978	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	73432	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	79362	63.476	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	126.960%
7) Chloroethane-d5	1.904	69	68204	62.372	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	124.740%
11) 1,1-Dichloroethene-d2	2.560	63	114562	49.801	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.600%
21) 2-Butanone-d5	4.615	46	124665	120.883	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.880%
24) Chloroform-d	5.052	84	158211	59.790	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.580%
26) 1,2-Dichloroethane-d4	5.692	65	105975	62.915	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	125.840%#
32) Benzene-d6	5.718	84	335090	64.609	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	129.220%#
36) 1,2-Dichloropropane-d6	6.682	67	103303	65.090	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	130.180%#
41) Toluene-d8	7.891	98	304394	63.040	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	126.080%#
43) trans-1,3-Dichloroprop...	8.171	79	48112	60.638	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	121.280%
47) 2-Hexanone-d5	8.624	63	94956	118.263	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	118.260%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	147307	58.973	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	117.940%
66) 1,2-Dichlorobenzene-d4	12.187	152	102691	63.172	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	126.340%#
Target Compounds						
37) 1,2-Dichloropropane	6.679	63	11015	9.015	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061282.D
Acq On : 29 Oct 2024 14:08
Operator : MD/SY
Sample : P4436-11
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Oct 29 22:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 29 22:33:34 2024
Response via : Initial Calibration

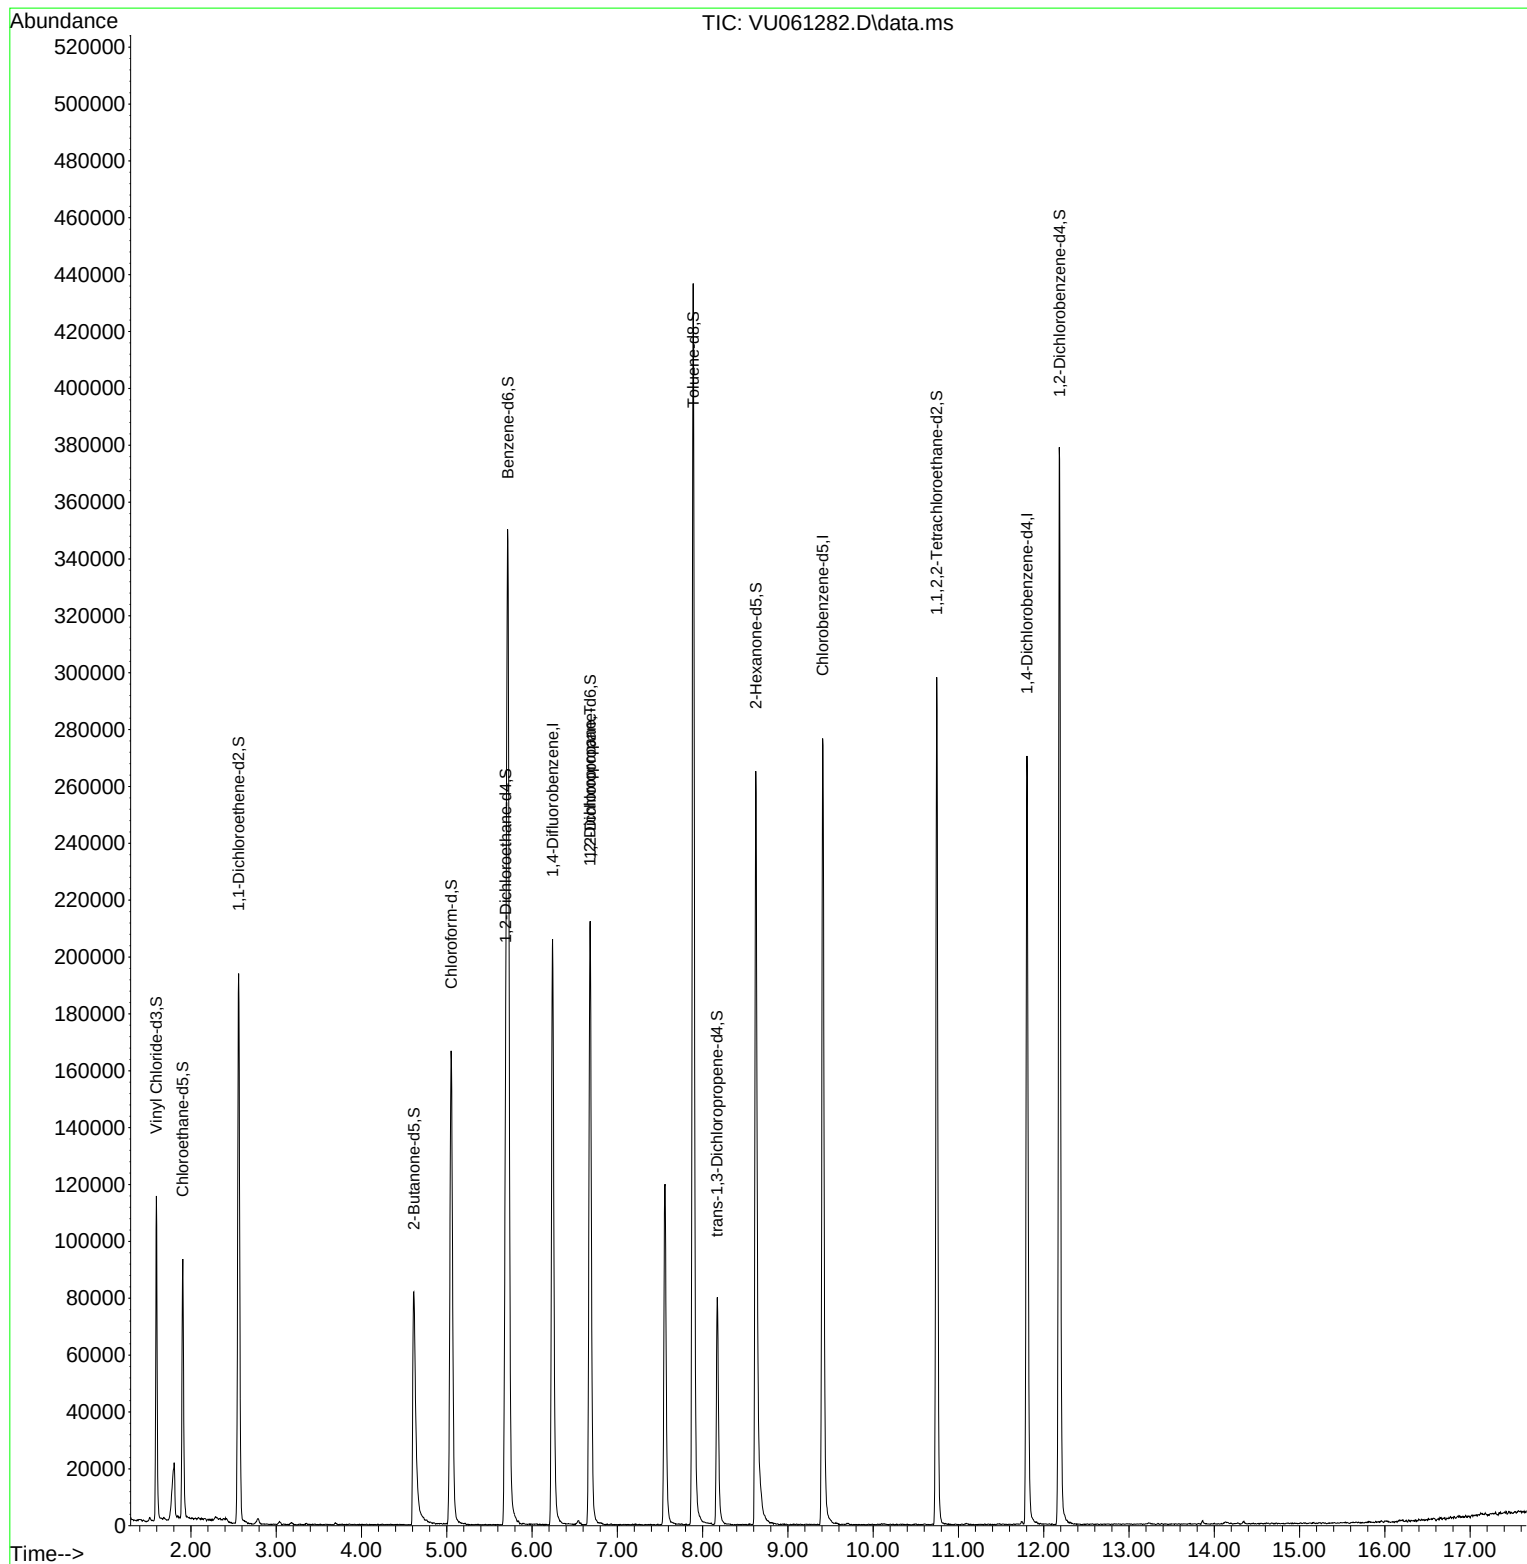

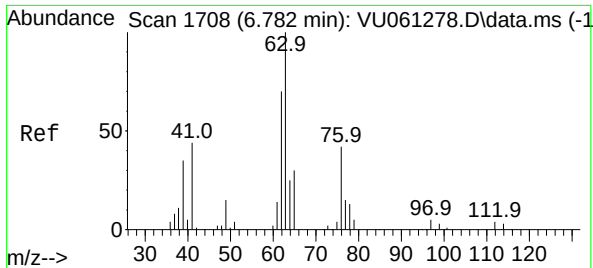

#37
1,2-Dichloropropane
Concen: 9.015 ug/L
RT: 6.679 min Scan# 1
Delta R.T. -0.103 min
Lab File: VU061282.D
Acq: 29 Oct 2024 14:08

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 11015
Ion Ratio Lower Upper
63 100
112 0.0 3.3 4.9#

