

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061290.D
 Acq On : 29 Oct 2024 17:18
 Operator : MD/SY
 Sample : VIBLK
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 29 22:36:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 29 22:33:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	253302	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	234859	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	105195	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	1174	0.660	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	1.320%#
7) Chloroethane-d5	1.904	69	526	0.338	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	0.680%#
11) 1,1-Dichloroethene-d2	2.560	63	2004	0.612	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	1.220%#
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	100.000	Range	40 - 130	Recovery	=	0.000%#
24) Chloroform-d	5.052	84	324	0.086	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	0.180%#
26) 1,2-Dichloroethane-d4	5.705	65	424	0.177	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	0.360%#
32) Benzene-d6	5.727	84	1404	0.187	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	0.380%#
36) 1,2-Dichloropropane-d6	6.682	67	134	0.058	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	0.120%#
41) Toluene-d8	7.901	98	2701	0.386	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	0.780%#
43) trans-1,3-Dichloroprop...	8.190	79	639	0.555	ug/L	0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	1.120%#
47) 2-Hexanone-d5	8.653	63	43	0.037	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	0.040%#
56) 1,1,2,2-Tetrachloroeth...	10.753	84	753	0.208	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	0.420%#
66) 1,2-Dichlorobenzene-d4	12.196	152	3395	1.458	ug/L	0.01
Spiked Amount	50.000	Range	80 - 120	Recovery	=	2.920%#
Target Compounds						
60) 1,2,3-Trichloropropane	11.804	75	13317	5.966	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061290.D
Acq On : 29 Oct 2024 17:18
Operator : MD/SY
Sample : VIBLK
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Oct 29 22:36:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 29 22:33:34 2024
Response via : Initial Calibration

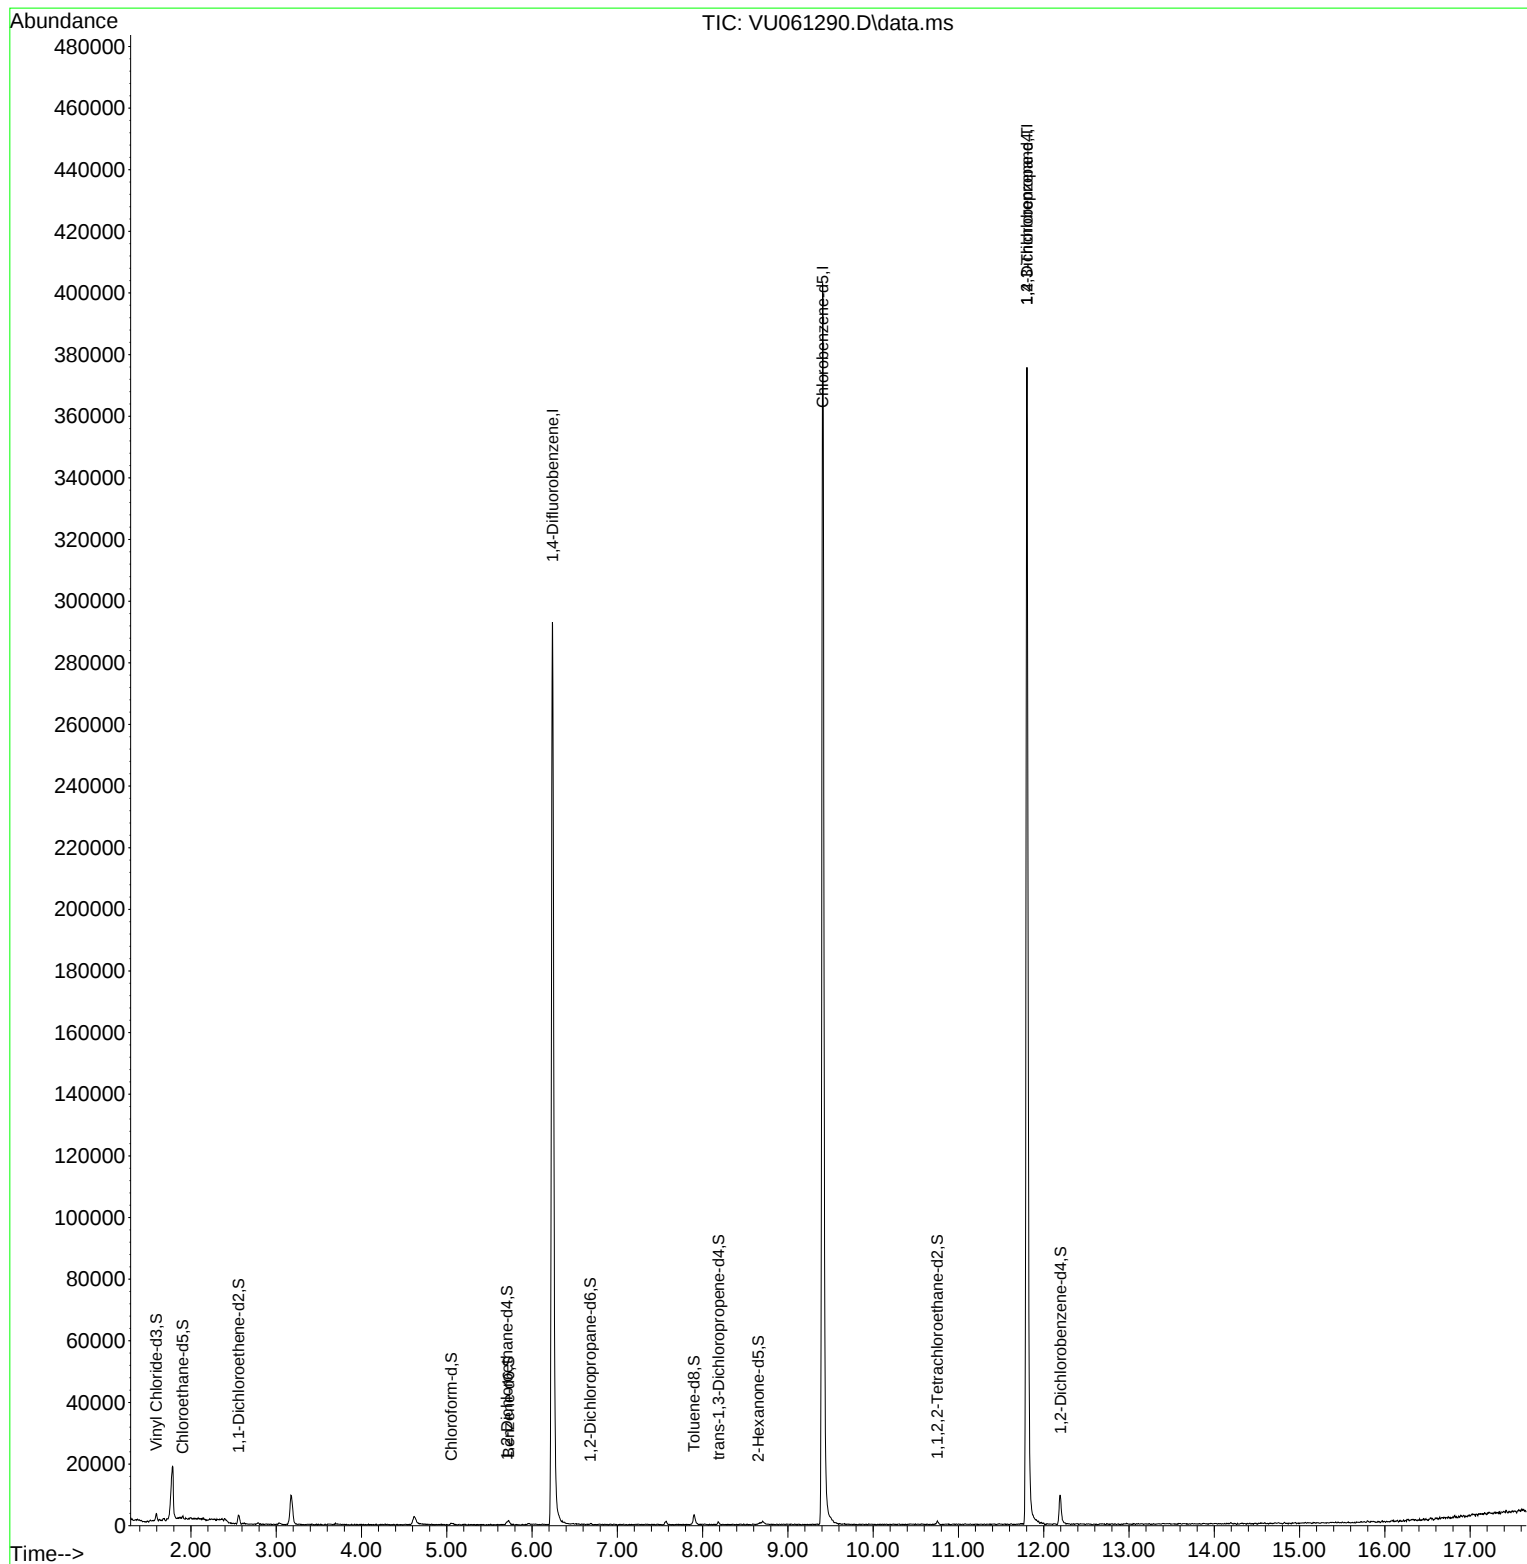

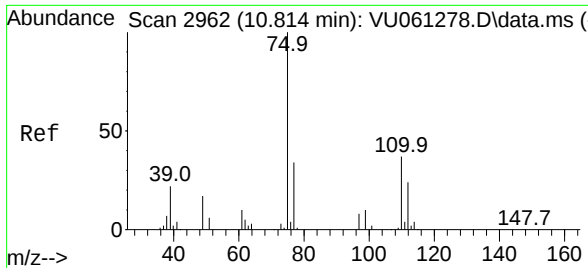

#60
 1,2,3-Trichloropropane
 Concen: 5.966 ug/L
 RT: 11.804 min Scan# 31
 Delta R.T. 0.990 min
 Lab File: VU061290.D
 Acq: 29 Oct 2024 17:18

Instrument :
 MSVOA_U
 ClientSampleId :

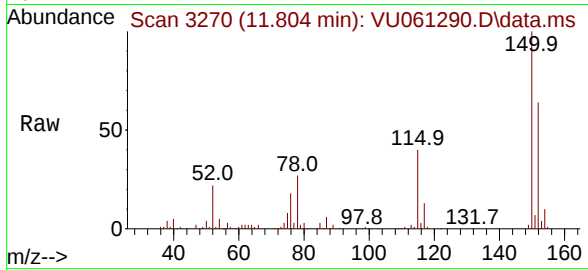

Tgt Ion:	75	Resp:	13317
Ion	Ratio	Lower	Upper
75	100		
77	34.1	25.5	38.3
110	2.7	29.8	44.6#

