

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061286.D
 Acq On : 29 Oct 2024 15:43
 Operator : MD/SY
 Sample : P4581-17
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4FK0

Quant Time: Oct 29 22:35:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 29 22:33:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	265115	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	245613	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	111506	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	76244	40.945	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.880%		
7) Chloroethane-d5	1.904	69	66179	40.635	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.260%		
11) 1,1-Dichloroethene-d2	2.560	63	112259	32.766	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.540%		
21) 2-Butanone-d5	4.611	46	122706	79.888	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.890%		
24) Chloroform-d	5.052	84	154539	39.213	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.420%		
26) 1,2-Dichloroethane-d4	5.692	65	102240	40.754	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.500%		
32) Benzene-d6	5.718	84	326225	41.481	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	6.679	67	100511	41.766	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.540%		
41) Toluene-d8	7.891	98	299769	40.942	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.880%		
43) trans-1,3-Dichloroprop...	8.171	79	47783	39.717	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.440%		
47) 2-Hexanone-d5	8.624	63	96322	79.114	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.110%		
56) 1,1,2,2-Tetrachloroeth...	10.746	84	145862	38.511	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	77.020%		
66) 1,2-Dichlorobenzene-d4	12.183	152	101071	40.946	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.900%		
Target Compounds						
					Qvalue	
13) Acetone	2.621	43	17484	15.450	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061286.D
Acq On : 29 Oct 2024 15:43
Operator : MD/SY
Sample : P4581-17
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4FK0

Quant Time: Oct 29 22:35:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 29 22:33:34 2024
Response via : Initial Calibration

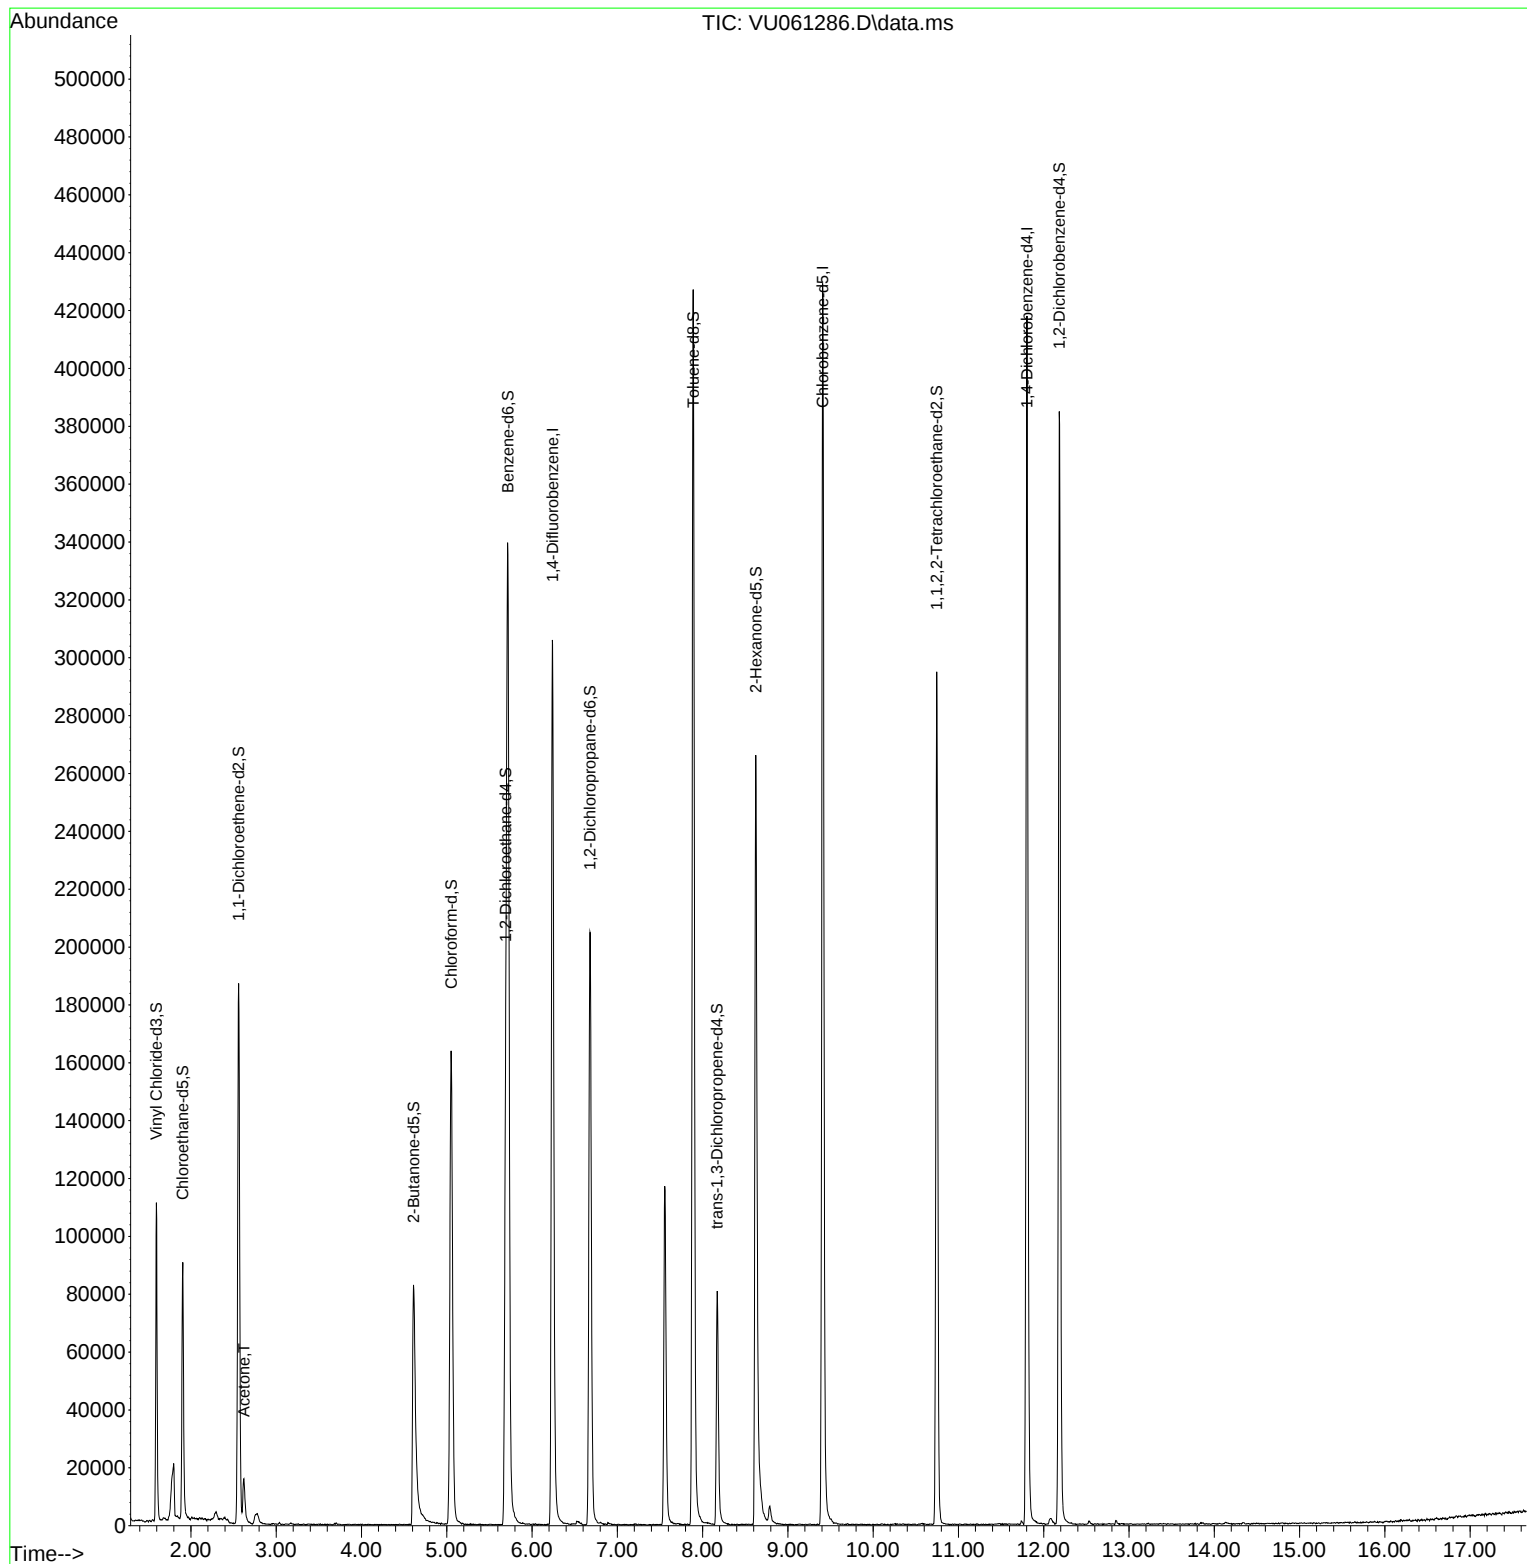

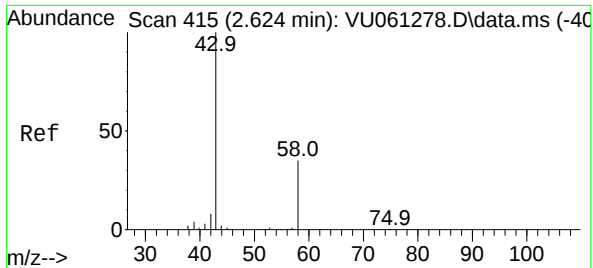

#13
 Acetone
 Concen: 15.450 ug/L
 RT: 2.621 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU061286.D
 Acq: 29 Oct 2024 15:43

Instrument :
 MSVOA_U
 ClientSampleId :
 A4FK0

Tgt Ion: 43 Resp: 17484
 Ion Ratio Lower Upper
 43 100
 58 36.1 0.0 68.2

