

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061275.D
 Acq On : 28 Oct 2024 19:31
 Operator : MD/SY
 Sample : VIBLK058
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

Signal : TIC: VU061275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.380	24	28	36	rBV4	1652	1820	0.18%	0.021%
2	1.515	65	70	80	rBV2	4943	6337	0.62%	0.072%
3	1.596	87	95	112	rBV	131415	155088	15.20%	1.763%
4	1.904	182	191	210	rVB	95033	131939	12.93%	1.500%
5	2.560	383	395	414	rBV	212302	358133	35.09%	4.071%
6	2.698	434	438	441	rBV3	316	279	0.03%	0.003%
7	2.785	454	465	484	rVB	20392	34427	3.37%	0.391%
8	2.875	489	493	498	rVB3	375	410	0.04%	0.005%
9	2.907	498	503	505	rBV	269	218	0.02%	0.002%
10	3.036	533	543	557	rVB3	5832	10970	1.07%	0.125%
11	3.178	574	587	602	rBV2	7471	17977	1.76%	0.204%
12	3.348	629	640	659	rVB2	14274	29108	2.85%	0.331%
13	3.689	736	746	747	rBV2	702	715	0.07%	0.008%
14	4.161	891	893	902	rVB2	200	293	0.03%	0.003%
15	4.200	902	905	909	rBV2	290	229	0.02%	0.003%
16	4.409	966	970	973	rBV	241	203	0.02%	0.002%
17	4.435	973	978	979	rVV2	255	185	0.02%	0.002%
18	4.477	988	991	997	rVB2	262	273	0.03%	0.003%
19	4.615	1024	1034	1075	rBV	85832	245507	24.06%	2.791%
20	4.965	1135	1143	1155	rBV5	4087	8350	0.82%	0.095%
21	5.052	1155	1170	1199	rVV	173178	389879	38.20%	4.432%
22	5.226	1220	1224	1228	rVB4	644	566	0.06%	0.006%
23	5.258	1231	1234	1235	rBV	283	188	0.02%	0.002%
24	5.280	1239	1241	1245	rBV	368	267	0.03%	0.003%
25	5.309	1245	1250	1252	rBV2	461	463	0.05%	0.005%
26	5.380	1261	1272	1284	rBV4	2927	6485	0.64%	0.074%
27	5.432	1284	1288	1291	rVB	227	198	0.02%	0.002%
28	5.451	1291	1294	1299	rBV2	293	223	0.02%	0.003%
29	5.515	1303	1314	1324	rVB3	986	1809	0.18%	0.021%
30	5.714	1356	1376	1417	rBV2	368337	1020528	100.00%	11.600%
31	5.862	1420	1422	1425	rVV3	374	174	0.02%	0.002%
32	5.968	1453	1455	1457	rBV2	276	200	0.02%	0.002%
33	6.120	1498	1502	1505	rBV2	240	227	0.02%	0.003%
34	6.239	1524	1539	1568	rBV	327188	635304	62.25%	7.221%
35	6.444	1599	1603	1605	rBV2	301	196	0.02%	0.002%
36	6.493	1612	1618	1619	rBV2	157	176	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061275.D
Acq On : 28 Oct 2024 19:31
Operator : MD/SY
Sample : VIBLK058
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Title : VOC Analysis

37	6.541	1621	1633	1646	rVV5	12683	25891	2.54%	0.294%
38	6.682	1664	1677	1693	rBV	220565	433032	42.43%	4.922%
39	6.878	1732	1738	1740	rBV	260	219	0.02%	0.002%
40	6.936	1750	1756	1760	rBV2	209	274	0.03%	0.003%
41	7.052	1787	1792	1798	rBV2	225	292	0.03%	0.003%
42	7.100	1798	1807	1816	rBV3	1638	2639	0.26%	0.030%
43	7.165	1824	1827	1832	rBV2	246	259	0.03%	0.003%
44	7.193	1832	1836	1839	rBV2	213	190	0.02%	0.002%
45	7.473	1915	1923	1927	rVB	283	331	0.03%	0.004%
46	7.560	1938	1950	1981	rBV	128116	249823	24.48%	2.840%
47	7.792	2013	2022	2034	rBV3	6502	12934	1.27%	0.147%
48	7.891	2040	2053	2070	rBV	457979	816133	79.97%	9.277%
49	8.174	2129	2141	2168	rBV	89565	172757	16.93%	1.964%
50	8.396	2203	2210	2219	rVB3	2696	3790	0.37%	0.043%
51	8.547	2249	2257	2271	rVB2	10319	16467	1.61%	0.187%
52	8.624	2271	2281	2329	rBV2	278147	568179	55.68%	6.458%
53	8.785	2329	2331	2332	rBV2	580	248	0.02%	0.003%
54	8.849	2349	2351	2355	rVB2	604	317	0.03%	0.004%
55	8.917	2361	2372	2382	rBV3	2859	5119	0.50%	0.058%
56	8.955	2382	2384	2387	rVB3	400	191	0.02%	0.002%
57	9.039	2407	2410	2413	rVB	322	228	0.02%	0.003%
58	9.065	2413	2418	2421	rBV	311	261	0.03%	0.003%
59	9.264	2475	2480	2483	rBV2	228	255	0.02%	0.003%
60	9.332	2497	2501	2505	rVB2	321	297	0.03%	0.003%
61	9.409	2512	2525	2552	rBV	441651	792640	77.67%	9.010%
62	9.566	2565	2574	2587	rVB2	11258	18249	1.79%	0.207%
63	9.692	2603	2613	2630	rVV2	11467	19516	1.91%	0.222%
64	9.872	2665	2669	2672	rBV2	282	268	0.03%	0.003%
65	10.113	2730	2744	2763	rBV6	14200	35078	3.44%	0.399%
66	10.184	2763	2766	2769	rVB3	410	260	0.03%	0.003%
67	10.283	2793	2797	2812	rVB5	1786	2772	0.27%	0.032%
68	10.480	2846	2858	2872	rBV	10700	17814	1.75%	0.202%
69	10.746	2924	2941	2957	rBV	311670	512396	50.21%	5.824%
70	10.885	2980	2984	2986	rBV2	375	280	0.03%	0.003%
71	11.084	3037	3046	3062	rVB2	12818	20271	1.99%	0.230%
72	11.406	3140	3146	3150	rVB2	223	263	0.03%	0.003%
73	11.463	3155	3164	3178	rBV	16881	26210	2.57%	0.298%
74	11.598	3201	3206	3207	rBV	274	174	0.02%	0.002%
75	11.740	3241	3250	3259	rBV	24608	39152	3.84%	0.445%
76	11.804	3259	3270	3295	rVB	429280	748768	73.37%	8.511%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061275.D
 Acq On : 28 Oct 2024 19:31
 Operator : MD/SY
 Sample : VIBLK058
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

77	11.988	3325	3327	3332	rVB3	309	212	0.02%	0.002%
78	12.016	3333	3336	3341	rBV2	205	179	0.02%	0.002%
79	12.184	3375	3388	3418	rBV	426253	735012	72.02%	8.355%
80	12.364	3438	3444	3445	rBV2	267	255	0.02%	0.003%
81	12.393	3450	3453	3457	rVV2	197	171	0.02%	0.002%
82	12.569	3503	3508	3510	rBV2	238	251	0.02%	0.003%
83	12.685	3541	3544	3550	rVB2	268	325	0.03%	0.004%
84	12.714	3550	3553	3556	rBV	271	182	0.02%	0.002%
85	12.759	3564	3567	3569	rVV2	329	216	0.02%	0.002%
86	12.785	3573	3575	3582	rVB2	315	270	0.03%	0.003%
87	12.840	3588	3592	3597	rBV	274	230	0.02%	0.003%
88	12.991	3631	3639	3652	rBV4	7442	12542	1.23%	0.143%
89	13.216	3699	3709	3728	rVB2	30999	52059	5.10%	0.592%
90	13.627	3833	3837	3841	rBV	325	333	0.03%	0.004%
91	13.746	3870	3874	3875	rBV	312	198	0.02%	0.002%
92	13.833	3891	3901	3918	rBV	57625	95283	9.34%	1.083%
93	14.081	3966	3978	4001	rBV	97306	180959	17.73%	2.057%
94	14.322	4043	4053	4074	rVB	67578	113480	11.12%	1.290%
95	14.483	4101	4103	4107	rVB2	376	258	0.03%	0.003%
96	14.608	4139	4142	4144	rBV2	300	217	0.02%	0.002%
97	14.884	4226	4228	4230	rBV2	313	208	0.02%	0.002%
98	15.524	4424	4427	4430	rBV2	323	280	0.03%	0.003%
99	15.817	4516	4518	4522	rBV2	516	445	0.04%	0.005%
100	16.232	4645	4647	4651	rBV3	608	371	0.04%	0.004%


Sum of corrected areas: 8797517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061275.D
Acq On : 28 Oct 2024 19:31
Operator : MD/SY
Sample : VIBLK058
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

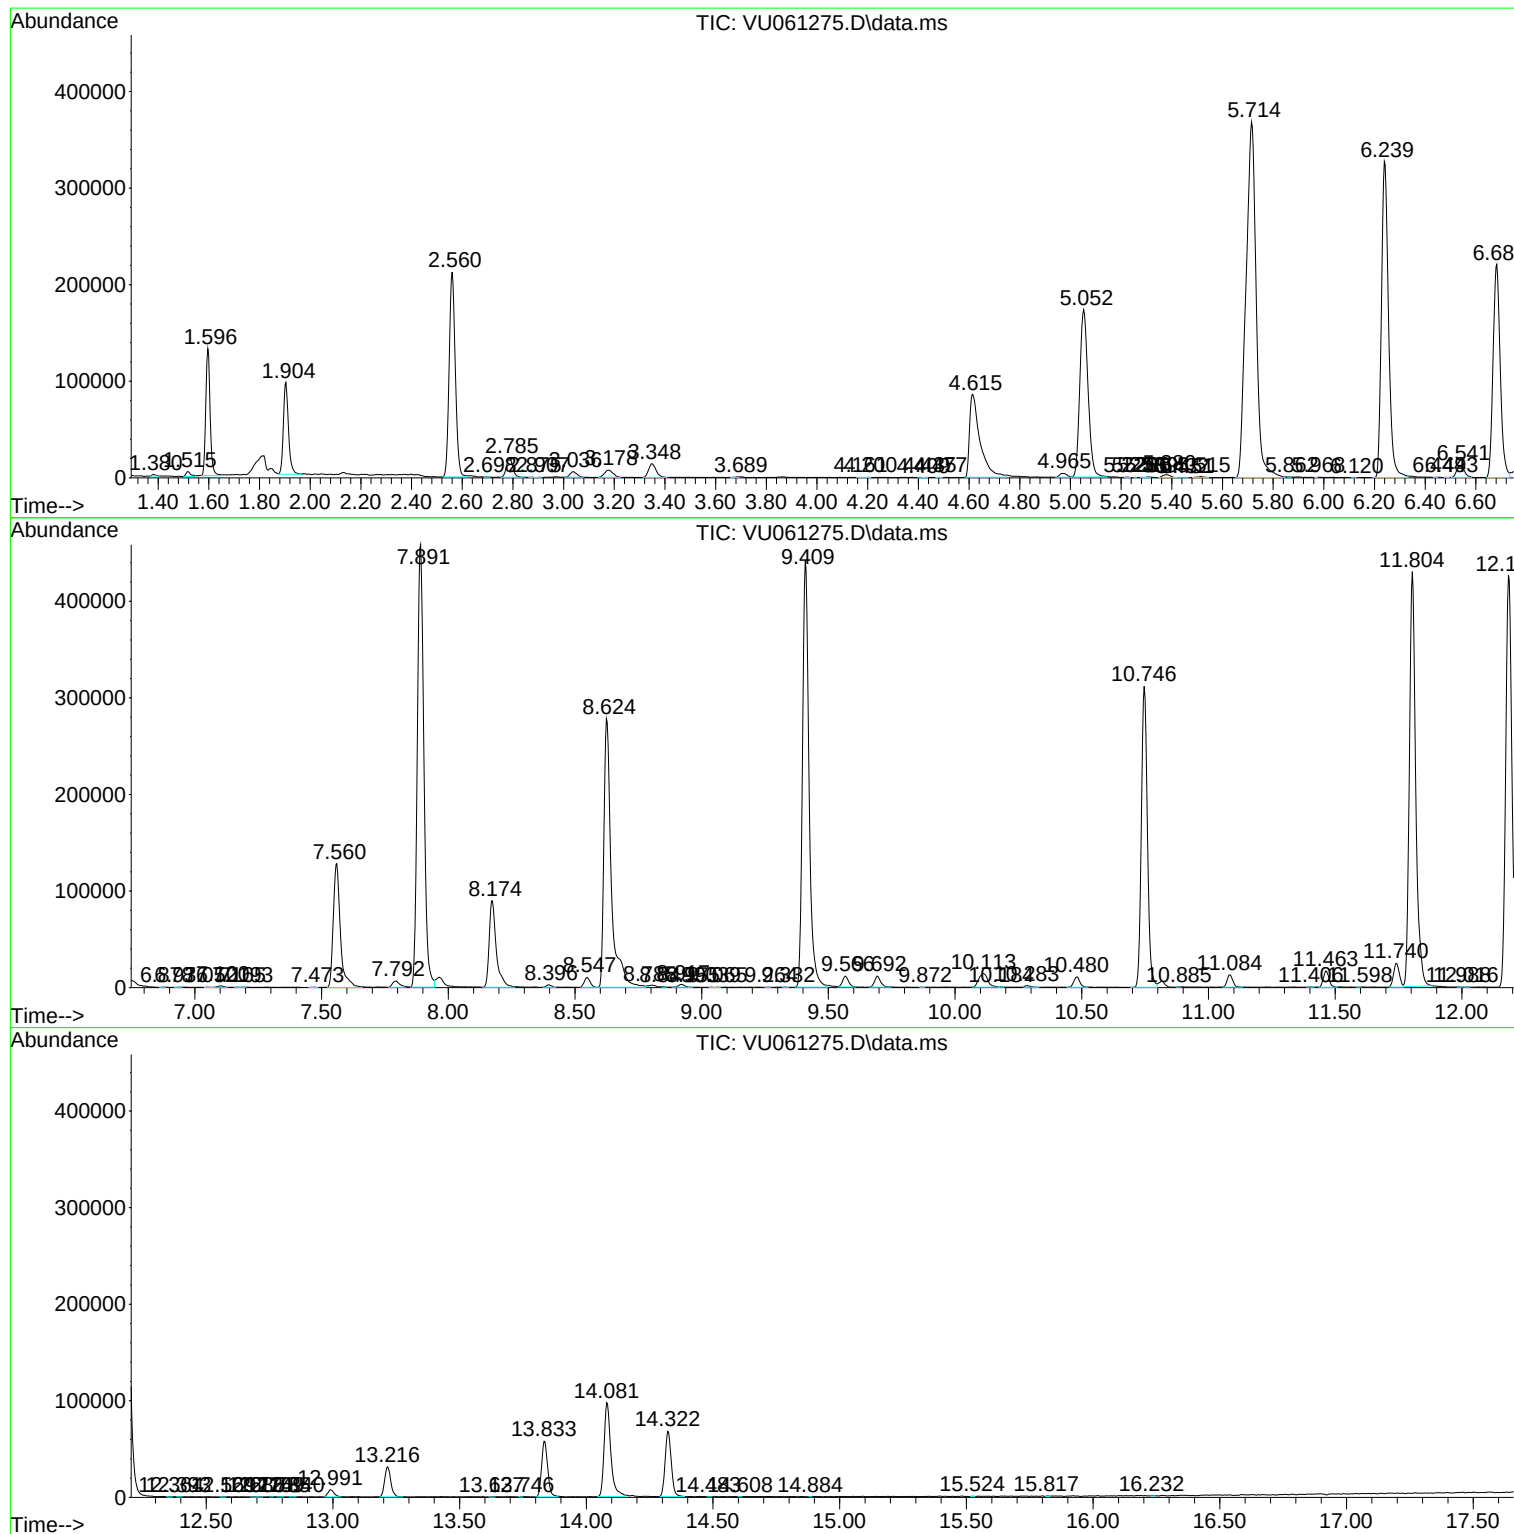

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061275.D
Acq On : 28 Oct 2024 19:31
Operator : MD/SY
Sample : VIBLK058
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061275.D
Acq On : 28 Oct 2024 19:31
Operator : MD/SY
Sample : VIBLK058
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK058

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------