

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061287.D
 Acq On : 29 Oct 2024 16:07
 Operator : MD/SY
 Sample : P4582-06
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M

Title : VOC Analysis

Signal : TIC: VU061287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rBV	116084	130974	13.51%	1.764%
2	1.904	183	191	209	rBV	90550	123298	12.71%	1.661%
3	2.560	383	395	407	rBV	193691	315305	32.51%	4.248%
4	2.753	446	455	476	rBV3	4080	9834	1.01%	0.132%
5	2.853	483	486	488	rBV	423	270	0.03%	0.004%
6	2.904	500	502	504	rBV	238	141	0.01%	0.002%
7	3.123	568	570	573	rBV2	166	105	0.01%	0.001%
8	3.171	581	585	589	rBV2	568	633	0.07%	0.009%
9	3.220	597	600	602	rBV	206	135	0.01%	0.002%
10	3.248	606	609	614	rVV	209	200	0.02%	0.003%
11	3.329	631	634	637	rVB2	234	147	0.02%	0.002%
12	3.416	658	661	665	rBV	174	121	0.01%	0.002%
13	3.483	677	682	686	rBV	188	246	0.03%	0.003%
14	3.525	692	695	699	rVB2	236	207	0.02%	0.003%
15	3.773	768	772	775	rVB	218	111	0.01%	0.001%
16	3.856	794	798	799	rBV	206	140	0.01%	0.002%
17	4.020	846	849	856	rVB2	346	388	0.04%	0.005%
18	4.104	873	875	879	rBV	206	165	0.02%	0.002%
19	4.126	879	882	886	rVB2	237	175	0.02%	0.002%
20	4.236	913	916	923	rBV2	277	406	0.04%	0.005%
21	4.342	947	949	952	rBV	161	128	0.01%	0.002%
22	4.445	977	981	985	rBV2	196	196	0.02%	0.003%
23	4.609	1023	1032	1072	rBV	84987	221893	22.88%	2.989%
24	5.052	1155	1170	1196	rBV	168599	377060	38.88%	5.079%
25	5.216	1219	1221	1224	rBV2	282	151	0.02%	0.002%
26	5.264	1234	1236	1238	rVB2	308	108	0.01%	0.001%
27	5.309	1248	1250	1253	rVB2	167	105	0.01%	0.001%
28	5.329	1254	1256	1260	rVB	140	119	0.01%	0.002%
29	5.348	1260	1262	1265	rBV	213	142	0.01%	0.002%
30	5.396	1274	1277	1281	rVB	188	118	0.01%	0.002%
31	5.428	1282	1287	1292	rVB2	276	201	0.02%	0.003%
32	5.464	1295	1298	1303	rVB2	170	153	0.02%	0.002%
33	5.496	1303	1308	1309	rBV	170	175	0.02%	0.002%
34	5.531	1315	1319	1324	rVB2	250	257	0.03%	0.003%
35	5.554	1324	1326	1328	rBV	177	106	0.01%	0.001%
36	5.628	1347	1349	1352	rBV2	147	114	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061287.D
 Acq On : 29 Oct 2024 16:07
 Operator : MD/SY
 Sample : P4582-06
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

37	5.715	1352	1376	1402	rBV2	354418	969734	100.00%	13.063%
38	6.094	1491	1494	1495	rBV2	274	113	0.01%	0.002%
39	6.123	1499	1503	1505	rVB	153	112	0.01%	0.002%
40	6.139	1505	1508	1511	rVB2	213	181	0.02%	0.002%
41	6.162	1511	1515	1518	rBV	213	204	0.02%	0.003%
42	6.181	1518	1521	1526	rBV2	193	201	0.02%	0.003%
43	6.239	1527	1539	1565	rBV	300327	589851	60.83%	7.946%
44	6.592	1646	1649	1651	rBV2	382	251	0.03%	0.003%
45	6.605	1651	1653	1656	rVB	210	134	0.01%	0.002%
46	6.628	1656	1660	1661	rBV	251	136	0.01%	0.002%
47	6.679	1663	1676	1704	rBV	212756	426147	43.94%	5.741%
48	6.994	1771	1774	1777	rVB	199	137	0.01%	0.002%
49	7.036	1778	1787	1792	rBV2	189	342	0.04%	0.005%
50	7.097	1801	1806	1807	rBV	147	105	0.01%	0.001%
51	7.161	1823	1826	1828	rBV	200	158	0.02%	0.002%
52	7.210	1836	1841	1844	rBV	226	294	0.03%	0.004%
53	7.358	1884	1887	1892	rBV2	259	252	0.03%	0.003%
54	7.415	1901	1905	1910	rBV2	240	267	0.03%	0.004%
55	7.499	1927	1931	1934	rBV2	136	133	0.01%	0.002%
56	7.557	1938	1949	1974	rBV	121926	222089	22.90%	2.992%
57	7.776	2015	2017	2020	rBV	166	121	0.01%	0.002%
58	7.888	2039	2052	2082	rBV	446348	792022	81.67%	10.669%
59	8.129	2124	2127	2130	rBV2	344	250	0.03%	0.003%
60	8.171	2130	2140	2163	rVV	82534	145183	14.97%	1.956%
61	8.361	2195	2199	2200	rBV2	233	138	0.01%	0.002%
62	8.444	2220	2225	2228	rBV2	217	267	0.03%	0.004%
63	8.570	2260	2264	2267	rVB	243	195	0.02%	0.003%
64	8.624	2270	2281	2315	rBV	271674	522185	53.85%	7.034%
65	8.965	2384	2387	2388	rBV	255	101	0.01%	0.001%
66	9.010	2398	2401	2404	rVB	230	133	0.01%	0.002%
67	9.065	2414	2418	2420	rBV	182	175	0.02%	0.002%
68	9.206	2460	2462	2465	rVB	210	129	0.01%	0.002%
69	9.316	2490	2496	2498	rBV	150	176	0.02%	0.002%
70	9.332	2499	2501	2503	rBV2	165	116	0.01%	0.002%
71	9.409	2513	2525	2564	rBV	421064	738549	76.16%	9.949%
72	9.682	2606	2610	2611	rBV	236	175	0.02%	0.002%
73	9.737	2623	2627	2630	rBV2	291	244	0.03%	0.003%
74	9.875	2666	2670	2672	rBV2	190	177	0.02%	0.002%
75	9.962	2693	2697	2699	rBV	189	165	0.02%	0.002%
76	10.142	2747	2753	2757	rBV2	399	470	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061287.D
 Acq On : 29 Oct 2024 16:07
 Operator : MD/SY
 Sample : P4582-06
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4FF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

77	10.190	2764	2768	2775	rBV2	230	324	0.03%	0.004%
78	10.267	2786	2792	2794	rBV2	400	339	0.03%	0.005%
79	10.296	2798	2801	2805	rBV2	364	312	0.03%	0.004%
80	10.428	2837	2842	2845	rVV2	182	187	0.02%	0.003%
81	10.480	2855	2858	2862	rVB	495	348	0.04%	0.005%
82	10.563	2883	2884	2885	rBV	322	110	0.01%	0.001%
83	10.747	2928	2941	2973	rVB	304568	494062	50.95%	6.656%
84	10.859	2974	2976	2979	rBV2	219	123	0.01%	0.002%
85	10.914	2991	2993	2999	rVB2	168	168	0.02%	0.002%
86	10.978	3010	3013	3017	rBV2	249	231	0.02%	0.003%
87	11.120	3054	3057	3060	rBV	228	198	0.02%	0.003%
88	11.171	3070	3073	3075	rBV2	173	124	0.01%	0.002%
89	11.345	3123	3127	3130	rVB2	224	230	0.02%	0.003%
90	11.364	3130	3133	3137	rBV2	291	219	0.02%	0.003%
91	11.393	3137	3142	3148	rVB2	285	363	0.04%	0.005%
92	11.467	3162	3165	3166	rBV2	254	138	0.01%	0.002%
93	11.602	3204	3207	3211	rVB	353	221	0.02%	0.003%
94	11.804	3258	3270	3291	rBV	408992	665517	68.63%	8.965%
95	12.081	3346	3356	3368	rBV6	2035	5150	0.53%	0.069%
96	12.184	3376	3388	3415	rBV	389285	657914	67.84%	8.863%
97	12.454	3470	3472	3476	rVB2	409	276	0.03%	0.004%
98	13.293	3730	3733	3736	rBV3	496	347	0.04%	0.005%
99	13.634	3837	3839	3841	rBV	302	141	0.01%	0.002%
100	14.348	4057	4061	4064	rBV3	566	369	0.04%	0.005%




Sum of corrected areas: 7423250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061287.D
Acq On : 29 Oct 2024 16:07
Operator : MD/SY
Sample : P4582-06
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

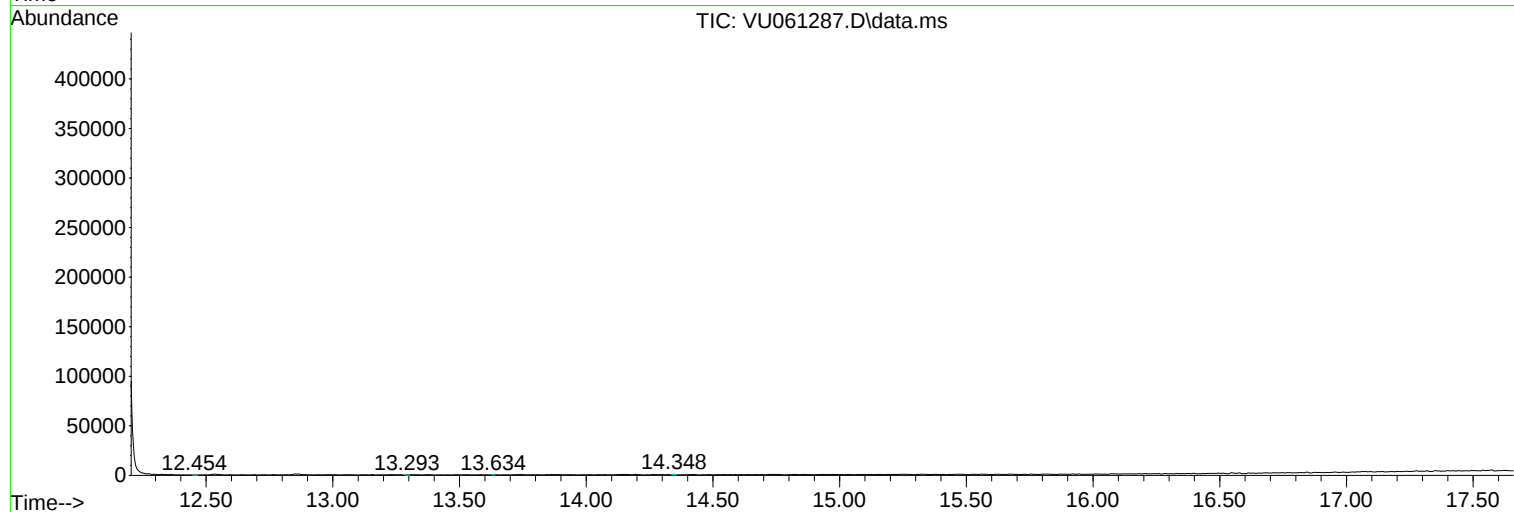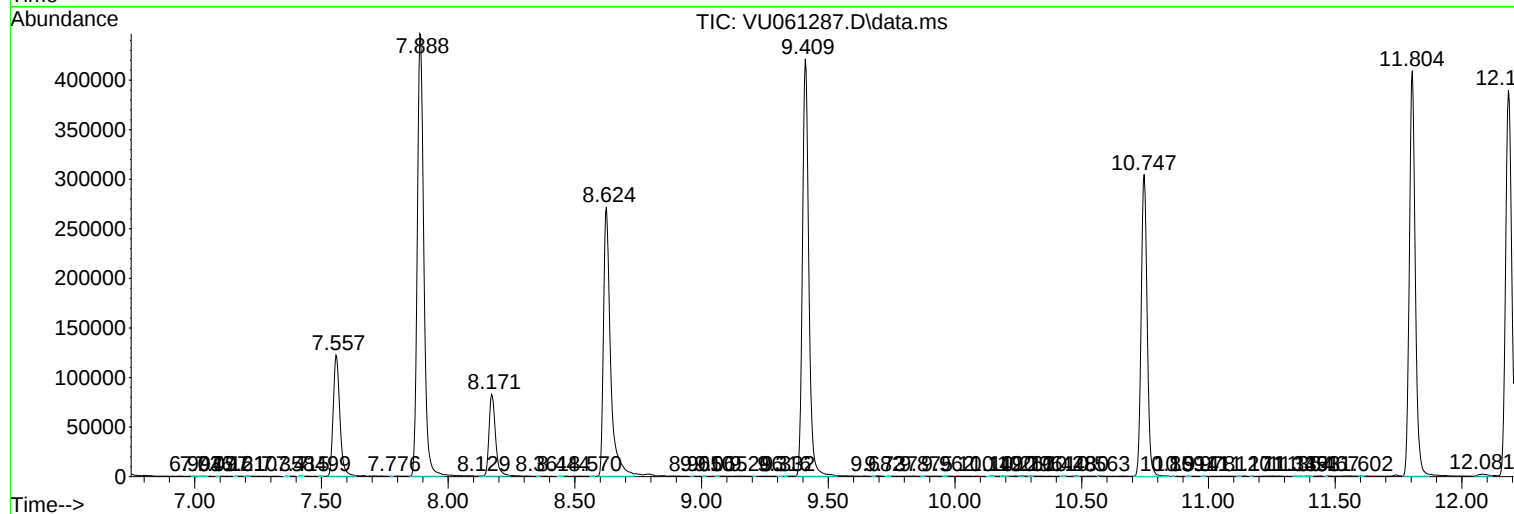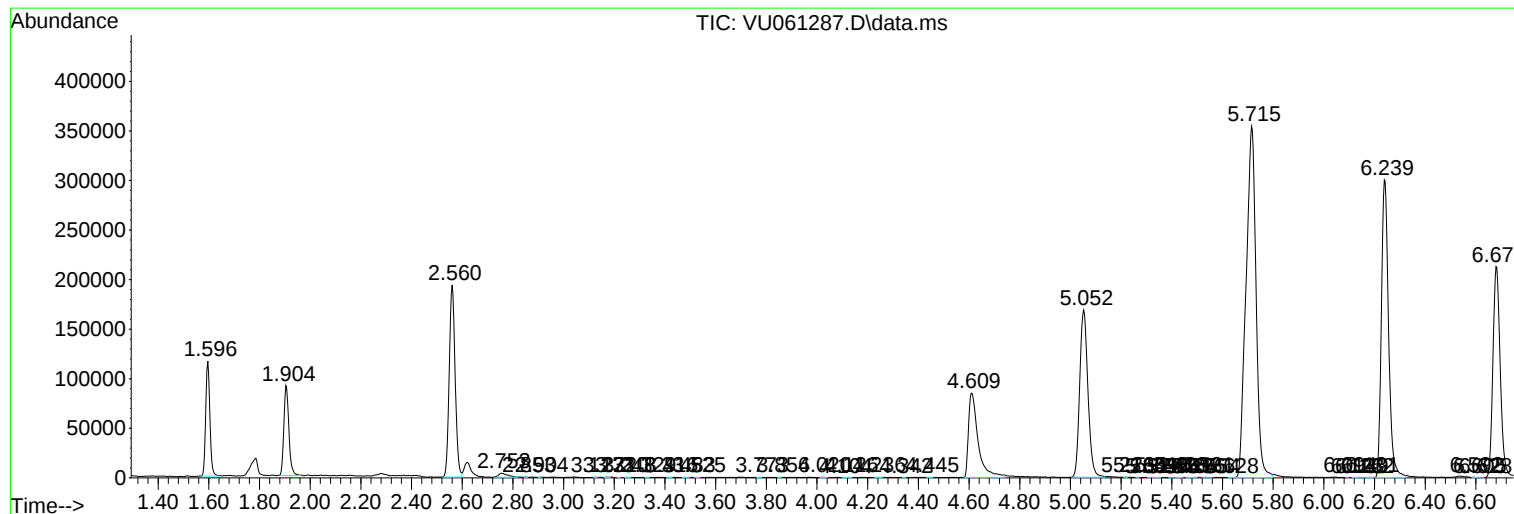

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061287.D
Acq On : 29 Oct 2024 16:07
Operator : MD/SY
Sample : P4582-06
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061287.D
Acq On : 29 Oct 2024 16:07
Operator : MD/SY
Sample : P4582-06
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4FF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------