

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061288.D
 Acq On : 29 Oct 2024 16:30
 Operator : MD/SY
 Sample : P4585-03
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M

Title : VOC Analysis

Signal : TIC: VU061288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	112	rBV	113822	128908	13.17%	1.744%
2	1.907	184	192	207	rBV	87074	120368	12.29%	1.628%
3	2.560	384	395	406	rBV	195509	316306	32.31%	4.279%
4	2.750	448	454	478	rVB2	5139	12088	1.23%	0.164%
5	2.997	527	531	538	rBV2	250	349	0.04%	0.005%
6	3.116	565	568	571	rBV	225	143	0.01%	0.002%
7	3.171	579	585	586	rBV3	1075	1109	0.11%	0.015%
8	3.399	654	656	659	rBV	222	161	0.02%	0.002%
9	3.435	664	667	673	rVB2	210	243	0.02%	0.003%
10	3.470	673	678	682	rBV	310	278	0.03%	0.004%
11	3.502	685	688	689	rBV2	180	104	0.01%	0.001%
12	3.541	697	700	702	rVB2	160	88	0.01%	0.001%
13	3.579	709	712	719	rVB2	307	312	0.03%	0.004%
14	3.608	719	721	722	rBV	237	122	0.01%	0.002%
15	3.997	839	842	844	rBV2	190	151	0.02%	0.002%
16	4.033	850	853	856	rBV2	208	170	0.02%	0.002%
17	4.139	883	886	888	rBV	133	79	0.01%	0.001%
18	4.187	897	901	905	rBV	227	220	0.02%	0.003%
19	4.312	934	940	942	rBV2	215	240	0.02%	0.003%
20	4.345	947	950	956	rVV2	225	195	0.02%	0.003%
21	4.415	970	972	976	rBV2	157	145	0.01%	0.002%
22	4.473	987	990	992	rBV2	229	147	0.02%	0.002%
23	4.525	1003	1006	1011	rBV	258	261	0.03%	0.004%
24	4.608	1023	1032	1063	rBV	82588	207412	21.19%	2.806%
25	5.052	1155	1170	1193	rBV	170741	380035	38.82%	5.142%
26	5.335	1256	1258	1259	rBV	121	45	0.00%	0.001%
27	5.357	1263	1265	1267	rBV	127	78	0.01%	0.001%
28	5.589	1334	1337	1339	rBV	216	148	0.02%	0.002%
29	5.634	1347	1351	1354	rVB	207	191	0.02%	0.003%
30	5.717	1356	1377	1412	rBV2	353360	979001	100.00%	13.245%
31	5.965	1451	1454	1457	rBV2	361	264	0.03%	0.004%
32	5.981	1457	1459	1463	rVV2	225	183	0.02%	0.002%
33	6.161	1512	1515	1517	rBV2	302	222	0.02%	0.003%
34	6.238	1527	1539	1564	rBV	300992	590583	60.33%	7.990%
35	6.615	1652	1656	1659	rBV2	514	390	0.04%	0.005%
36	6.631	1659	1661	1663	rVB	196	96	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061288.D
 Acq On : 29 Oct 2024 16:30
 Operator : MD/SY
 Sample : P4585-03
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

37	6.682	1663	1677	1705	rBV	215843	430090	43.93%	5.819%
38	6.888	1738	1741	1742	rBV2	693	407	0.04%	0.006%
39	6.991	1771	1773	1774	rBV	187	63	0.01%	0.001%
40	7.039	1785	1788	1791	rBV	101	77	0.01%	0.001%
41	7.065	1794	1796	1798	rVB	119	52	0.01%	0.001%
42	7.078	1798	1800	1803	rBV	139	105	0.01%	0.001%
43	7.139	1817	1819	1821	rBV2	123	72	0.01%	0.001%
44	7.177	1827	1831	1836	rBV2	238	236	0.02%	0.003%
45	7.380	1889	1894	1897	rVB2	205	175	0.02%	0.002%
46	7.422	1905	1907	1910	rBV	143	86	0.01%	0.001%
47	7.483	1924	1926	1930	rVB2	302	214	0.02%	0.003%
48	7.502	1930	1932	1934	rBV	74	48	0.00%	0.001%
49	7.512	1934	1935	1937	rBV	132	41	0.00%	0.001%
50	7.557	1938	1949	1972	rBV	120385	222484	22.73%	3.010%
51	7.705	1990	1995	1999	rBV3	462	576	0.06%	0.008%
52	7.759	2007	2012	2015	rBV2	206	172	0.02%	0.002%
53	7.785	2015	2020	2023	rBV3	272	268	0.03%	0.004%
54	7.843	2035	2038	2040	rBV	192	97	0.01%	0.001%
55	7.891	2040	2053	2081	rBV	448188	803233	82.05%	10.867%
56	8.174	2130	2141	2165	rBV	81516	144524	14.76%	1.955%
57	8.512	2244	2246	2249	rBV	168	139	0.01%	0.002%
58	8.624	2270	2281	2322	rBV	258345	513251	52.43%	6.944%
59	8.917	2370	2372	2375	rBV2	289	151	0.02%	0.002%
60	9.036	2406	2409	2410	rBV	320	183	0.02%	0.002%
61	9.087	2420	2425	2428	rBV2	279	271	0.03%	0.004%
62	9.106	2428	2431	2436	rBV2	160	172	0.02%	0.002%
63	9.241	2467	2473	2477	rBV2	272	344	0.04%	0.005%
64	9.261	2477	2479	2482	rBV	209	137	0.01%	0.002%
65	9.335	2500	2502	2505	rVB	169	68	0.01%	0.001%
66	9.357	2505	2509	2510	rBV2	244	186	0.02%	0.003%
67	9.409	2513	2525	2560	rBV	420411	728777	74.44%	9.860%
68	9.704	2612	2617	2621	rBV3	623	690	0.07%	0.009%
69	9.836	2653	2658	2661	rVB2	223	179	0.02%	0.002%
70	9.968	2696	2699	2702	rVB	226	145	0.01%	0.002%
71	10.016	2712	2714	2720	rBV	190	156	0.02%	0.002%
72	10.058	2720	2727	2729	rBV2	203	302	0.03%	0.004%
73	10.161	2756	2759	2761	rBV	195	158	0.02%	0.002%
74	10.299	2800	2802	2805	rVB	152	42	0.00%	0.001%
75	10.331	2805	2812	2815	rBV2	287	386	0.04%	0.005%
76	10.457	2849	2851	2854	rBV	242	169	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
 Data File : VU061288.D
 Acq On : 29 Oct 2024 16:30
 Operator : MD/SY
 Sample : P4585-03
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

77	10.566	2883	2885	2886	rBV	274	134	0.01%	0.002%
78	10.746	2928	2941	2960	rBV	303893	494658	50.53%	6.692%
79	10.839	2969	2970	2971	rBV	195	57	0.01%	0.001%
80	10.849	2971	2973	2976	rVB3	360	186	0.02%	0.003%
81	10.939	2998	3001	3003	rVB	255	126	0.01%	0.002%
82	10.955	3004	3006	3009	rBV2	232	150	0.02%	0.002%
83	11.200	3079	3082	3084	rBV	235	143	0.01%	0.002%
84	11.277	3102	3106	3110	rBV2	258	297	0.03%	0.004%
85	11.714	3240	3242	3245	rBV	480	274	0.03%	0.004%
86	11.804	3258	3270	3302	rBV	394174	653091	66.71%	8.836%
87	12.074	3347	3354	3362	rBV5	3209	5973	0.61%	0.081%
88	12.183	3376	3388	3411	rBV	376674	643866	65.77%	8.711%
89	12.524	3492	3494	3495	rBV	450	199	0.02%	0.003%
90	12.765	3566	3569	3577	rBV3	410	588	0.06%	0.008%
91	12.859	3595	3598	3600	rBV2	247	135	0.01%	0.002%
92	12.936	3618	3622	3624	rBV	466	310	0.03%	0.004%
93	13.537	3807	3809	3811	rBV	286	150	0.02%	0.002%
94	14.135	3990	3995	3998	rBV2	428	486	0.05%	0.007%
95	14.196	4009	4014	4019	rBV	320	462	0.05%	0.006%
96	14.293	4041	4044	4046	rBV	294	192	0.02%	0.003%
97	14.498	4105	4108	4110	rBV2	296	199	0.02%	0.003%




Sum of corrected areas: 7391437

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061288.D
Acq On : 29 Oct 2024 16:30
Operator : MD/SY
Sample : P4585-03
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

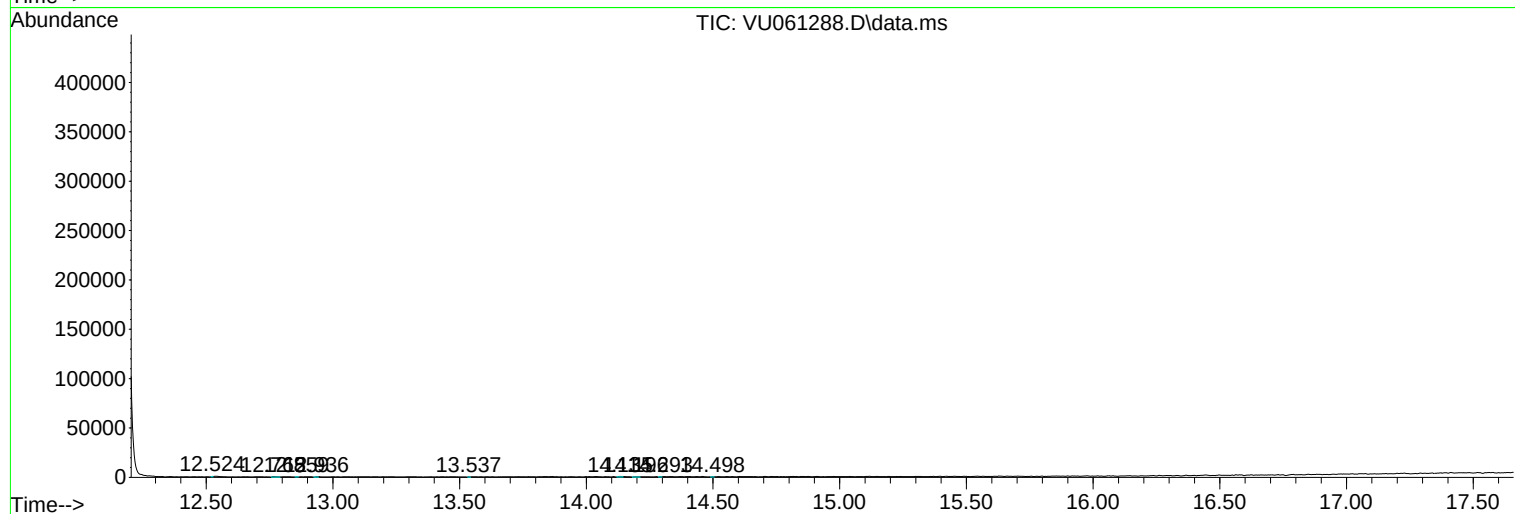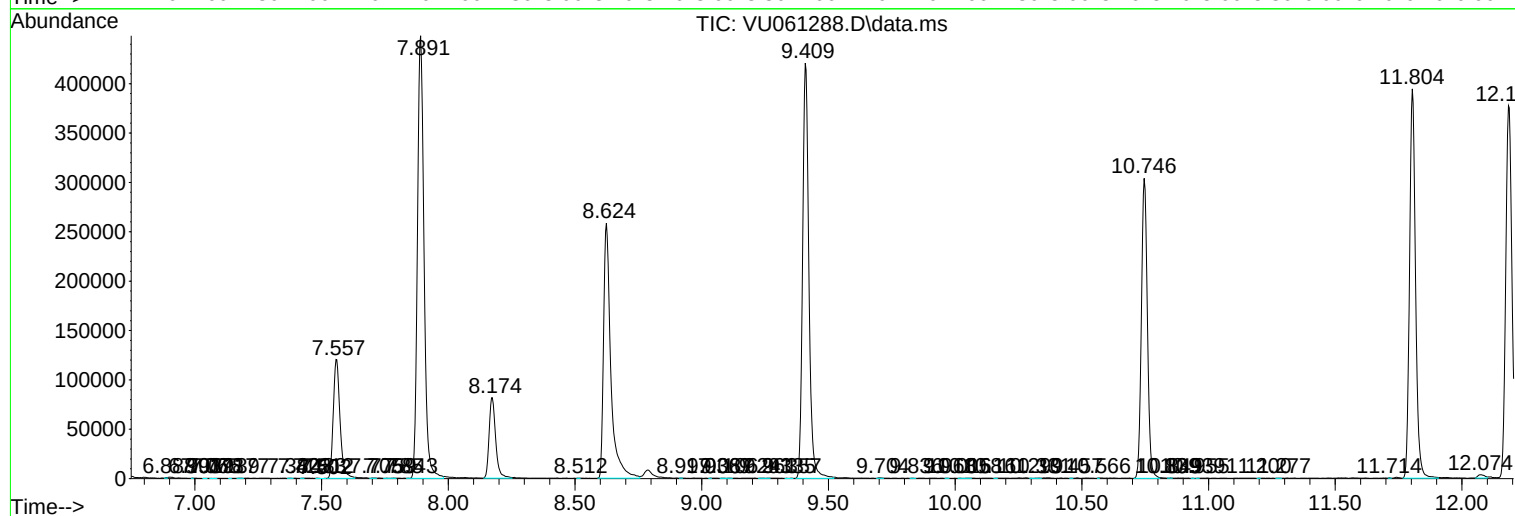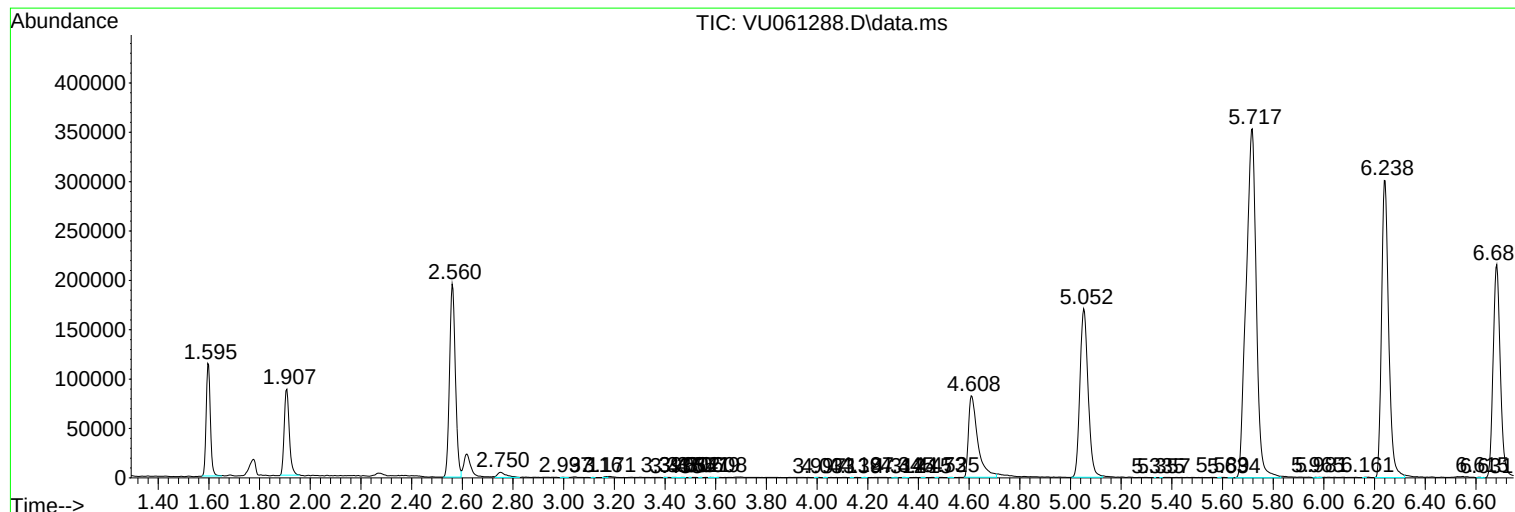

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061288.D
Acq On : 29 Oct 2024 16:30
Operator : MD/SY
Sample : P4585-03
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061288.D
Acq On : 29 Oct 2024 16:30
Operator : MD/SY
Sample : P4585-03
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------