
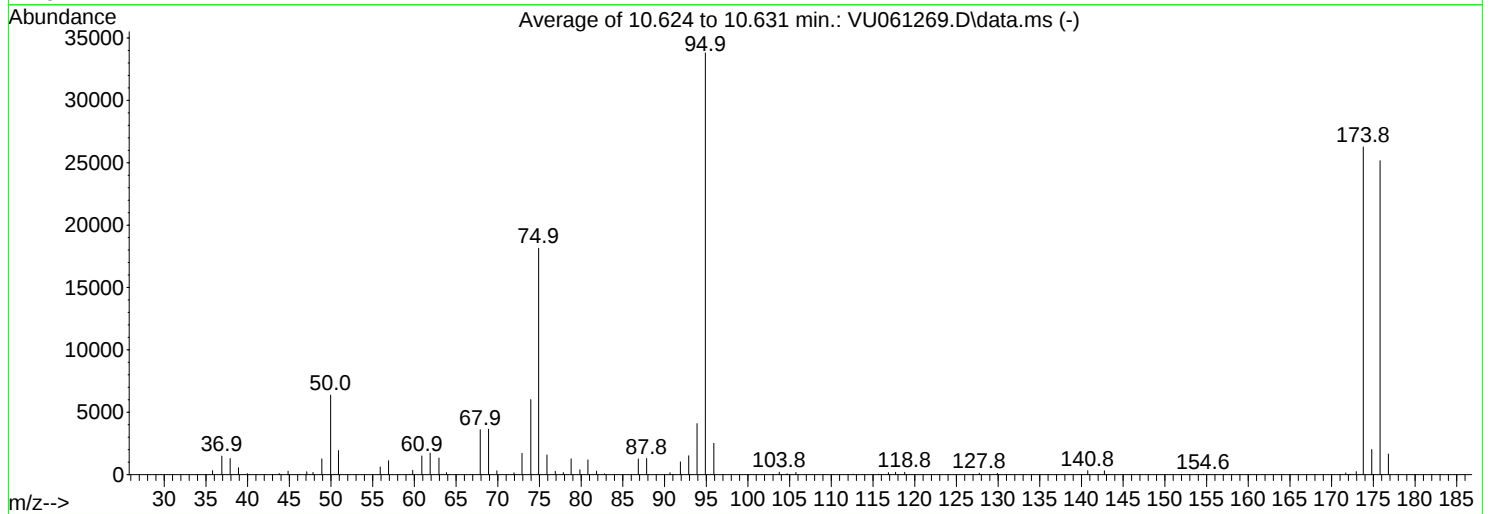


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061269.D
Acq On : 28 Oct 2024 16:24
Operator : MD/SY
Sample : BFB077
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB077

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Title : VOC Analysis
Last Update : Tue Oct 29 22:33:34 2024

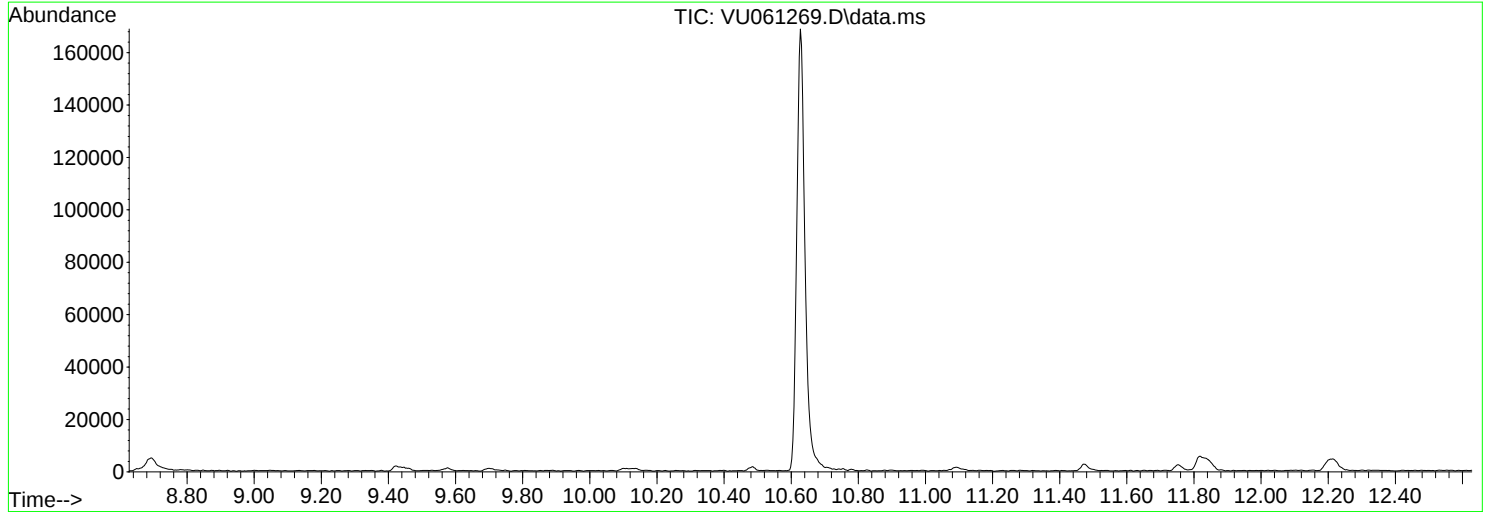

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	6380	PASS
75	95	30	80	53.7	18144	PASS
95	95	100	100	100.0	33808	PASS
96	95	5	9	7.5	2519	PASS
173	174	0.00	2	0.9	247	PASS
174	95	50	120	77.7	26264	PASS
175	174	5	9	7.7	2019	PASS
176	174	95	101	95.8	25160	PASS
177	176	5	9	6.6	1656	PASS

m/z	Abundance
43.80	510.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
35.80	281.0
36.90	1503.0
37.90	1266.0
38.90	505.0
40.00	148.0
43.80	593.0
44.90	281.0
47.10	219.0
47.90	211.0
48.90	1222.0
49.90	6243.0
50.90	2005.0
55.90	605.0
56.90	1142.0
59.80	327.0
60.90	1554.0
61.90	1799.0
62.90	1182.0
63.80	155.0
67.90	3704.0
68.90	3625.0
69.90	299.0
72.00	140.0
72.90	1747.0
73.90	6173.0
74.90	18088.0
75.90	1428.0
76.90	235.0
77.80	185.0
78.80	1251.0
79.80	348.0
80.80	1198.0
81.80	262.0
86.80	1267.0
87.90	1308.0
90.60	123.0
91.90	904.0
92.90	1316.0
93.90	3917.0
94.90	32488.0
95.90	2513.0
103.70	175.0
105.80	145.0
116.80	158.0
117.70	194.0
118.80	158.0
127.80	112.0
129.90	155.0
140.70	266.0
142.70	287.0
171.70	121.0
173.00	237.0
173.80	25072.0
174.80	1915.0
175.80	24216.0
176.80	1444.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
35.80	335.0
36.90	1570.0
37.90	1333.0
38.90	567.0
39.90	115.0
43.80	604.0
44.90	291.0
47.10	239.0
47.90	179.0
48.90	1309.0
50.00	6536.0
50.90	1973.0
55.90	628.0
56.90	1166.0
59.80	369.0
60.90	1537.0
61.90	1825.0
63.00	1380.0
63.80	185.0
67.90	3670.0
68.90	3764.0
69.90	320.0
72.00	148.0
72.90	1802.0
74.00	6162.0
74.90	18776.0
75.90	1647.0
76.90	279.0
77.80	178.0
78.80	1272.0
79.80	408.0
80.80	1212.0
81.90	304.0
82.80	111.0
86.80	1267.0
87.80	1286.0
90.60	154.0
91.90	1072.0
92.90	1590.0
93.90	4189.0
94.90	34920.0
95.90	2641.0
103.80	204.0
104.70	133.0
105.70	195.0
112.60	106.0
116.90	157.0
117.70	204.0
118.80	204.0
127.70	128.0
129.90	140.0
140.80	327.0
142.80	320.0
154.60	101.0
171.70	149.0
172.90	247.0
173.80	27176.0
174.80	2099.0
175.80	26080.0
176.80	1715.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
35.80	354.0
36.90	1409.0
37.90	1298.0
38.90	599.0
43.90	597.0
44.80	279.0
47.10	231.0
47.80	133.0
48.90	1262.0
49.90	6362.0
50.90	1793.0
55.90	619.0
56.90	1056.0
59.80	340.0
60.90	1396.0
61.90	1581.0
63.00	1421.0
63.90	166.0
67.90	3424.0
68.90	3559.0
69.90	287.0
71.90	160.0
72.90	1585.0
74.00	5697.0
74.90	17568.0
75.90	1679.0
76.90	304.0
77.90	142.0
78.80	1285.0
79.90	401.0
80.80	1113.0
81.90	286.0
82.80	102.0
86.90	1237.0
87.90	1288.0
90.70	168.0
91.90	1108.0
92.90	1652.0
93.90	4174.0
94.90	34016.0
95.90	2403.0
103.80	184.0
104.70	114.0
105.80	198.0
115.70	109.0
116.90	172.0
117.70	173.0
118.80	229.0
127.70	124.0
140.80	361.0
142.80	330.0
171.70	141.0
172.20	121.0
172.90	258.0
173.80	26544.0
174.80	2042.0
175.80	25184.0
176.80	1809.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077