
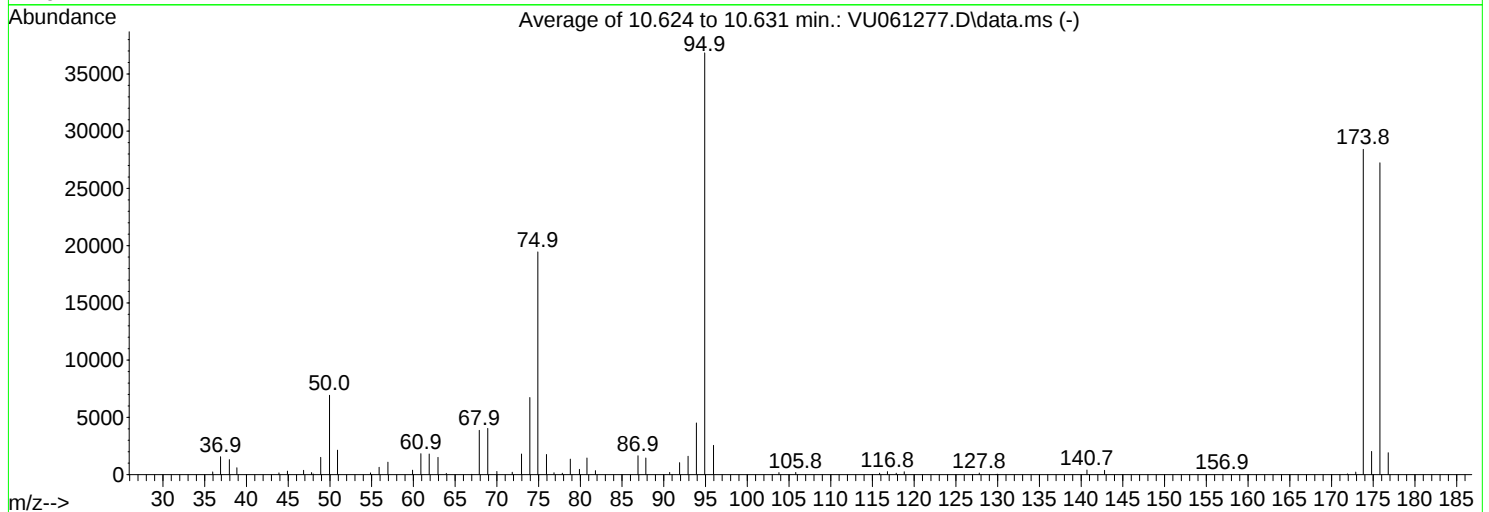


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102924\
Data File : VU061277.D
Acq On : 29 Oct 2024 09:59
Operator : MD/SY
Sample : BFB078
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB078

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Title : VOC Analysis
Last Update : Tue Oct 29 22:33:34 2024

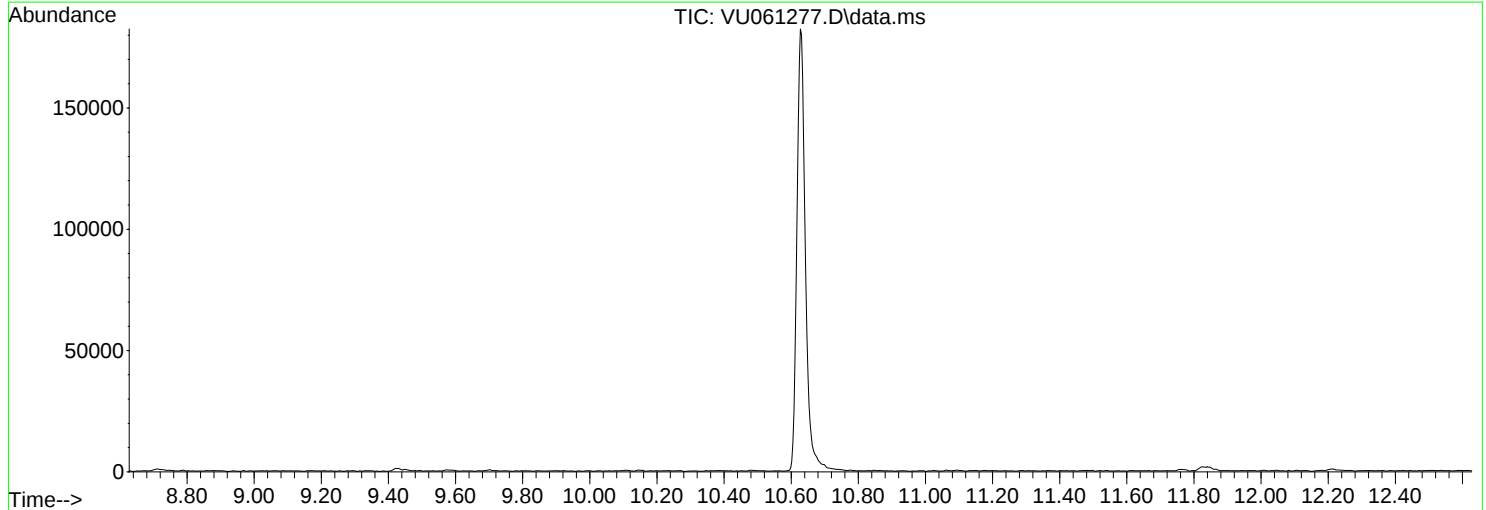

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	6930	PASS
75	95	30	80	52.8	19448	PASS
95	95	100	100	100.0	36840	PASS
96	95	5	9	6.9	2556	PASS
173	174	0.00	2	0.8	228	PASS
174	95	50	120	77.1	28419	PASS
175	174	5	9	7.1	2026	PASS
176	174	95	101	95.8	27232	PASS
177	176	5	9	7.0	1917	PASS

m/z	Abundance
39.80	177.0
43.90	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
35.90	251.0
36.90	1592.0
38.00	1334.0
38.80	605.0
39.90	128.0
43.90	468.0
44.90	263.0
46.80	346.0
47.80	151.0
48.00	151.0
48.90	1506.0
50.00	7024.0
50.90	2073.0
54.80	160.0
55.90	597.0
57.00	1078.0
59.90	350.0
60.90	1882.0
61.90	1758.0
62.90	1478.0
64.00	106.0
67.90	3734.0
68.90	3892.0
70.00	277.0
71.90	193.0
72.90	1547.0
73.90	6657.0
74.90	18528.0
75.90	1664.0
76.80	161.0
77.80	121.0
78.80	1277.0
79.90	495.0
80.80	1363.0
81.80	362.0
86.90	1416.0
87.80	1425.0
90.70	192.0
91.90	980.0
92.90	1608.0
93.90	4349.0
94.90	35216.0
95.90	2560.0
103.80	160.0
105.80	173.0
116.80	231.0
117.90	129.0
118.80	243.0
127.80	148.0
129.80	105.0
140.70	344.0
142.80	393.0
156.90	101.0
171.90	129.0
172.90	200.0
173.80	26104.0
174.80	1962.0
175.80	26032.0
176.80	1877.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
35.90	252.0
36.90	1638.0
37.90	1322.0
38.90	594.0
39.90	123.0
43.90	486.0
44.90	304.0
46.90	390.0
47.80	186.0
48.90	1574.0
50.00	7122.0
50.90	2200.0
54.90	150.0
55.90	666.0
56.90	1102.0
59.90	399.0
60.90	1876.0
61.90	1857.0
62.90	1561.0
64.00	127.0
67.90	4012.0
68.90	4143.0
70.00	293.0
71.80	224.0
73.00	1858.0
73.90	6892.0
74.90	20120.0
76.00	1852.0
76.80	167.0
77.90	134.0
78.80	1383.0
79.90	466.0
80.80	1501.0
81.80	356.0
86.90	1718.0
87.90	1457.0
90.70	209.0
91.90	1075.0
92.90	1639.0
93.90	4590.0
94.90	37944.0
95.90	2624.0
103.80	178.0
105.80	201.0
115.80	163.0
116.80	271.0
117.90	118.0
118.80	276.0
127.80	136.0
140.70	439.0
142.80	394.0
171.90	102.0
172.90	229.0
173.80	29416.0
174.80	2071.0
175.80	27960.0
176.80	1973.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078

m/z	Abundance
36.00	231.0
36.90	1483.0
37.90	1279.0
38.90	608.0
39.90	114.0
43.90	526.0
44.90	347.0
46.90	418.0
47.80	200.0
48.90	1438.0
49.90	6643.0
50.90	2153.0
54.90	134.0
55.90	674.0
56.90	1074.0
59.90	433.0
60.90	1733.0
61.90	1802.0
63.00	1482.0
63.90	116.0
67.00	103.0
67.90	3876.0
68.90	4069.0
70.00	269.0
71.80	231.0
73.00	1989.0
74.00	6645.0
74.90	19696.0
76.00	1772.0
76.90	170.0
77.80	118.0
78.80	1416.0
79.90	414.0
80.80	1488.0
81.80	346.0
86.90	1823.0
87.90	1468.0
90.70	186.0
91.90	1104.0
92.90	1563.0
93.90	4619.0
94.90	37360.0
96.00	2485.0
103.80	214.0
105.80	203.0
115.90	203.0
116.80	283.0
117.80	133.0
118.80	256.0
127.80	130.0
130.00	108.0
140.70	448.0
142.80	363.0
172.90	255.0
173.80	29736.0
174.80	2046.0
175.80	27704.0
176.80	1901.0

Instrument :
MSVOA_U
ClientSampleId :
BFB078