

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
 Data File : VU061336.D
 Acq On : 01 Nov 2024 02:16
 Operator : MD/SY
 Sample : P4631-21
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP15

Quant Time: Nov 01 04:10:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 01 00:44:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.241	114	172515	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	154972	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	68331	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	43095	3.677	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.600%
7) Chloroethane-d5	1.910	69	45845	4.267	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.400%
11) 1,1-Dichloroethene-d2	2.560	65	20630	4.115	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%
20) 2-Butanone-d5	4.624	46	116401	48.922	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.840%
24) Chloroform-d	5.052	84	101384	4.558	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.695	65	52528	4.738	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.717	84	210432	4.819	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
36) 1,2-Dichloropropane-d6	6.682	67	64595	4.920	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.891	98	191957	4.701	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	8.174	79	22053	4.115	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.627	63	97187	44.279	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.560%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	46678	4.702	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	60638	5.011	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds					Qvalue	
13) Acetone	2.644	43	14529	9.641	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061336.D
Acq On : 01 Nov 2024 02:16
Operator : MD/SY
Sample : P4631-21
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP15

Quant Time: Nov 01 04:10:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 01 00:44:02 2024
Response via : Initial Calibration

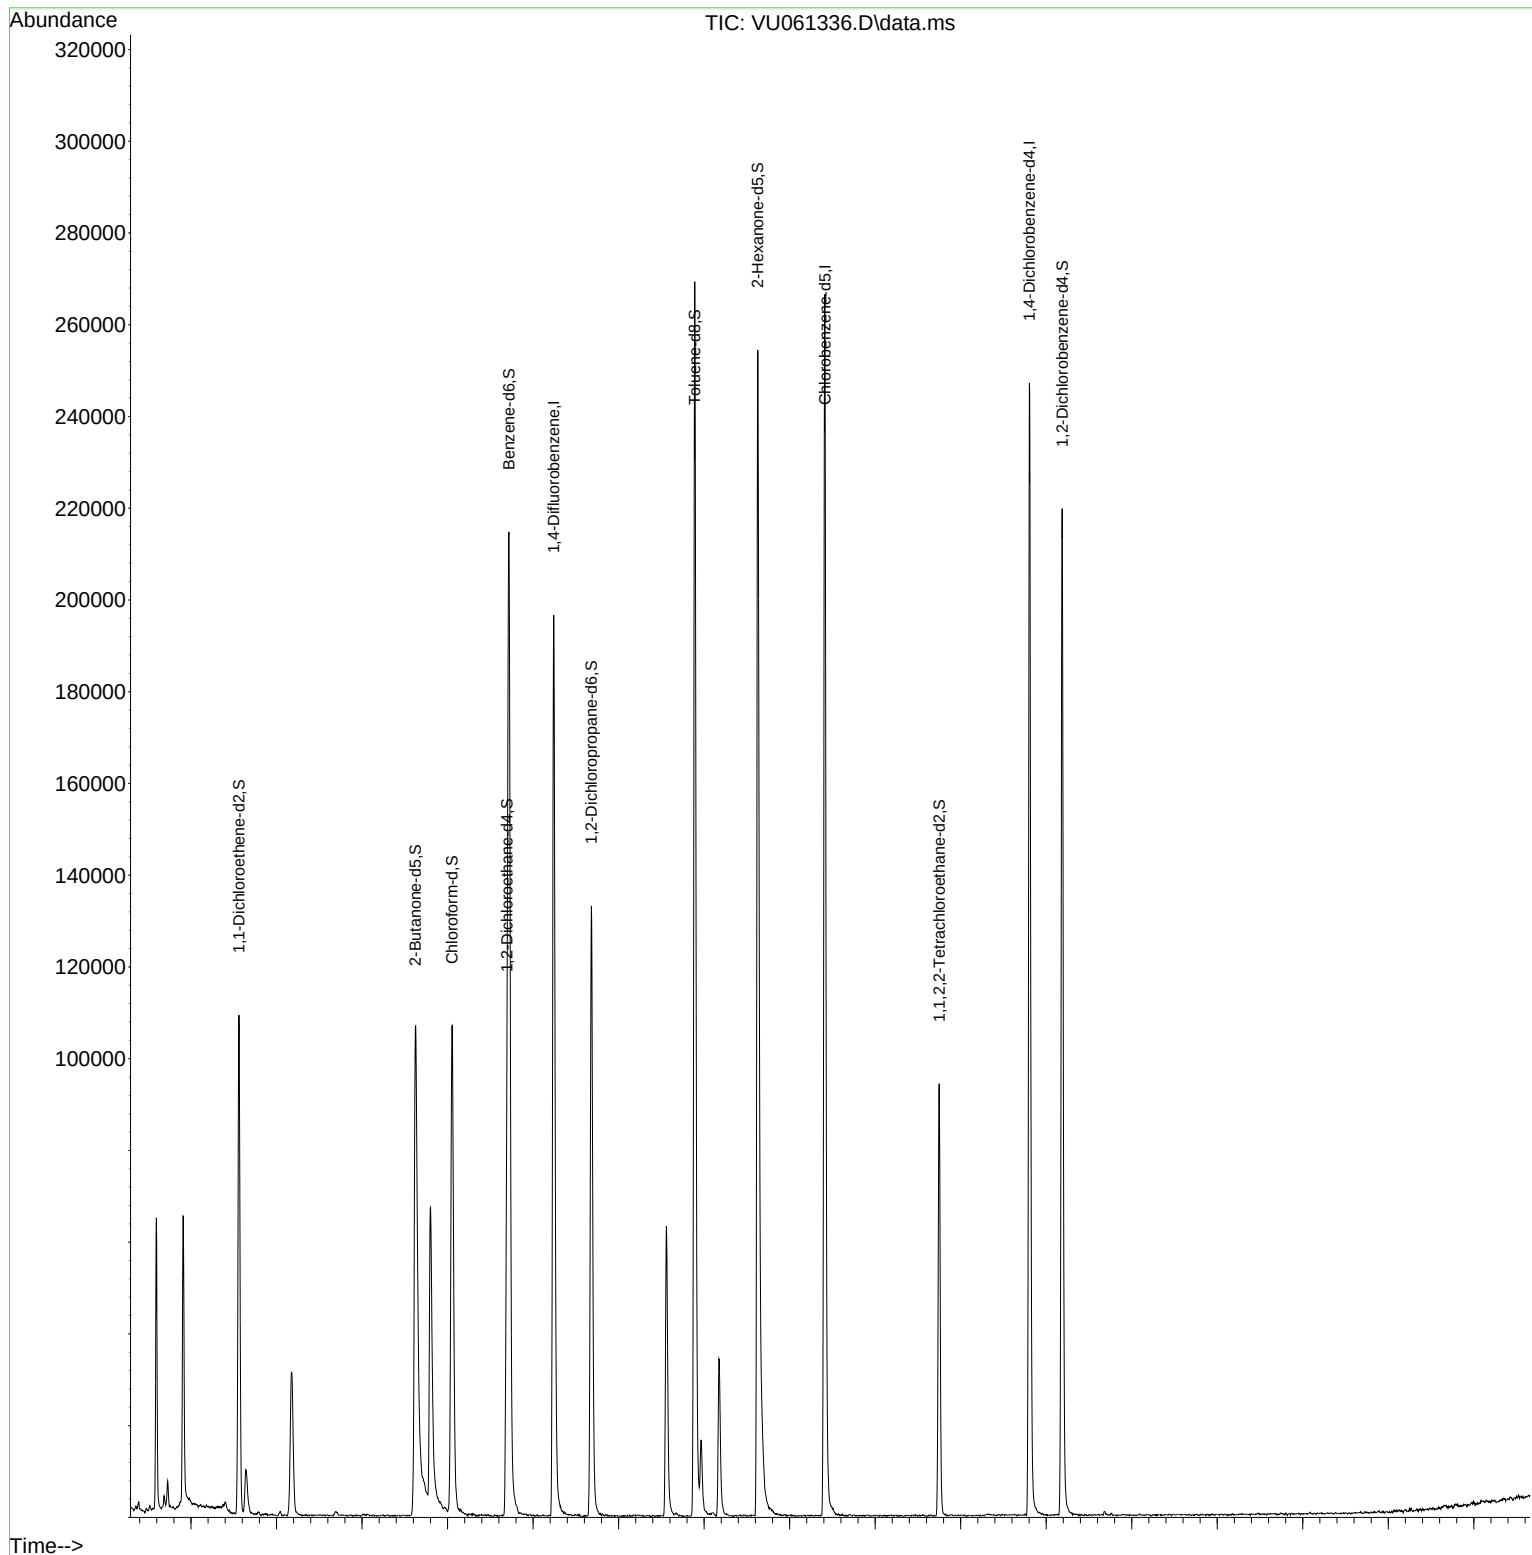

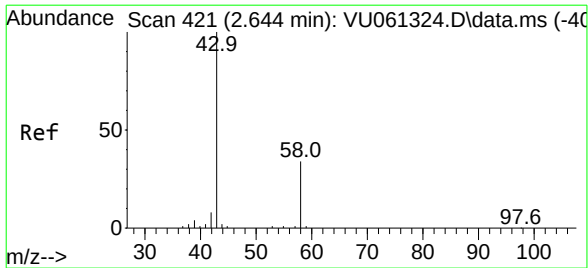

#13
 Acetone
 Concen: 9.641 ug/L
 RT: 2.644 min Scan# 42
 Delta R.T. -0.000 min
 Lab File: VU061336.D
 Acq: 01 Nov 2024 02:16

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP15

Tgt Ion:	43	Resp:	14529
Ion	Ratio	Lower	Upper
43	100		
58	32.7	0.0	73.2

