

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
 Data File : VU061312.D
 Acq On : 31 Oct 2024 15:26
 Operator : MD/SY
 Sample : VIBLK152
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK152

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rVB	80692	90174	14.84%	1.793%
2	1.911	183	193	206	rBV	71575	99845	16.43%	1.986%
3	2.560	384	395	413	rBV	128603	211234	34.76%	4.201%
4	3.177	572	587	603	rBV	9061	20224	3.33%	0.402%
5	4.628	1024	1038	1077	rBV	81640	233763	38.47%	4.649%
6	5.055	1156	1171	1194	rBV	112048	251344	41.36%	4.999%
7	5.718	1358	1377	1404	rBV2	232199	607674	100.00%	12.086%
8	6.242	1528	1540	1571	rBV	196915	383088	63.04%	7.619%
9	6.682	1660	1677	1706	rBV	138001	276177	45.45%	5.493%
10	7.560	1939	1950	1975	rBV2	68759	129398	21.29%	2.574%
11	7.891	2040	2053	2075	rBV	289602	519965	85.57%	10.341%
12	8.174	2131	2141	2161	rBV	40794	73157	12.04%	1.455%
13	8.627	2271	2282	2318	rBV2	267277	563740	92.77%	11.212%
14	9.412	2513	2526	2565	rBV	264907	473589	77.93%	9.419%
15	9.569	2565	2575	2588	rVB2	3670	6328	1.04%	0.126%
16	9.692	2605	2613	2626	rBV2	4262	7026	1.16%	0.140%
17	10.749	2929	2942	2961	rBV	95949	159310	26.22%	3.168%
18	11.807	3258	3271	3295	rBV	255842	444377	73.13%	8.838%
19	12.187	3374	3389	3414	rBV	232619	417946	68.78%	8.312%
20	13.839	3893	3903	3927	rBV3	30982	59618	9.81%	1.186%

Sum of corrected areas: 5027977




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061312.D
Acq On : 31 Oct 2024 15:26
Operator : MD/SY
Sample : VIBLK152
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

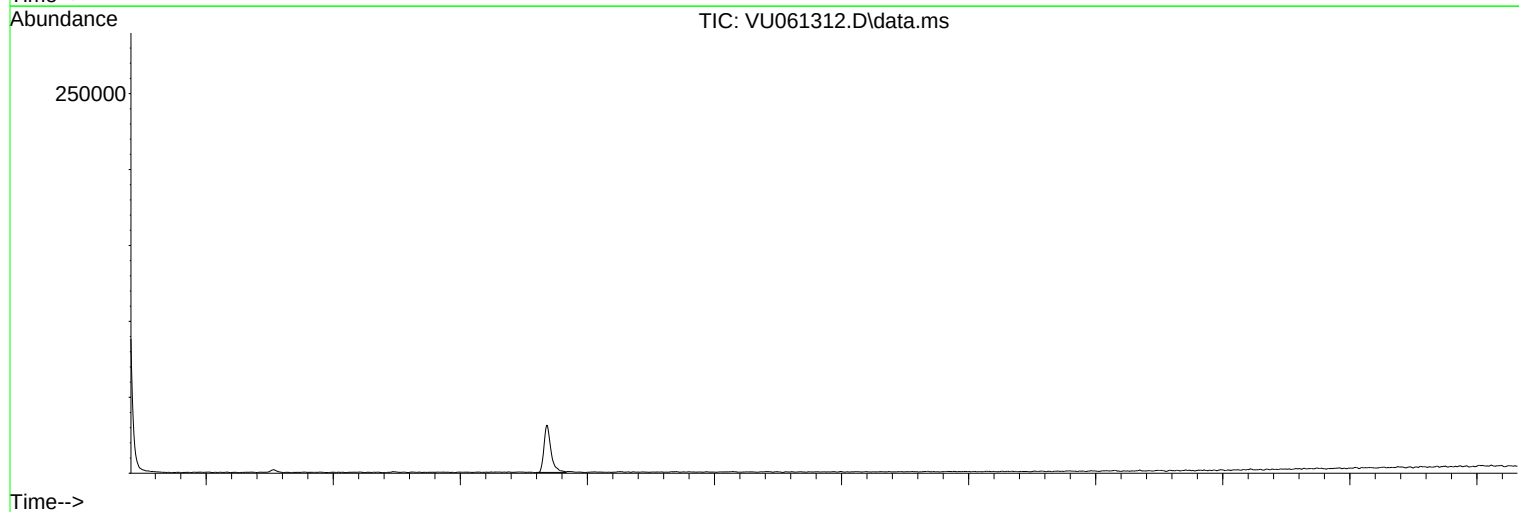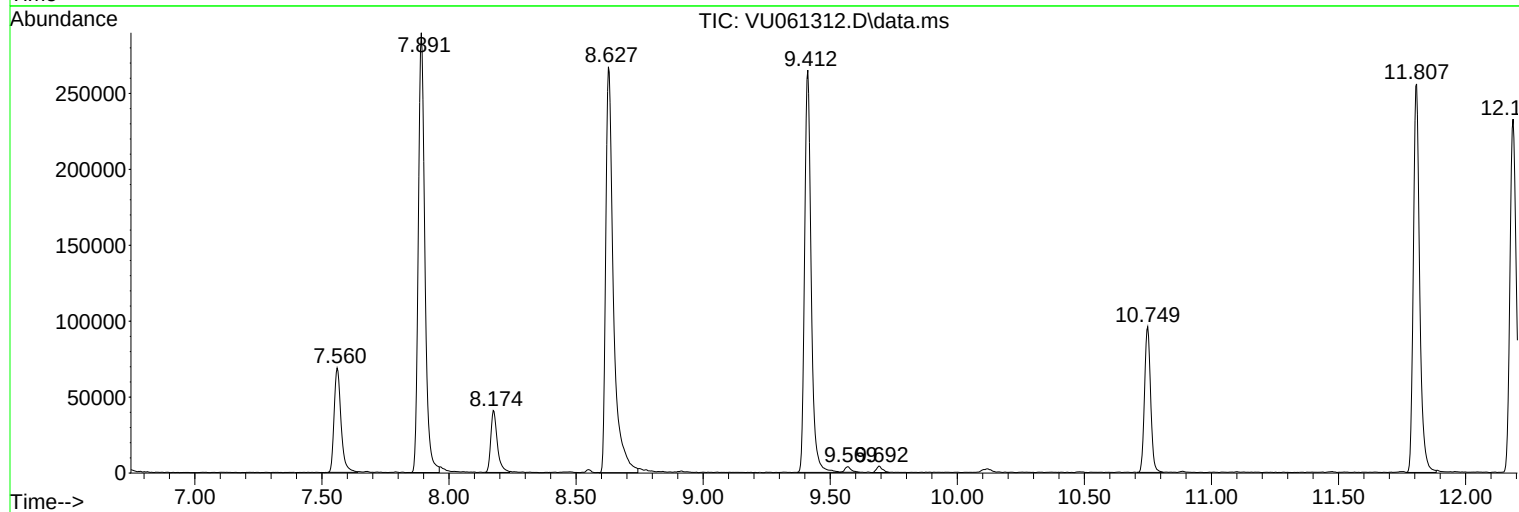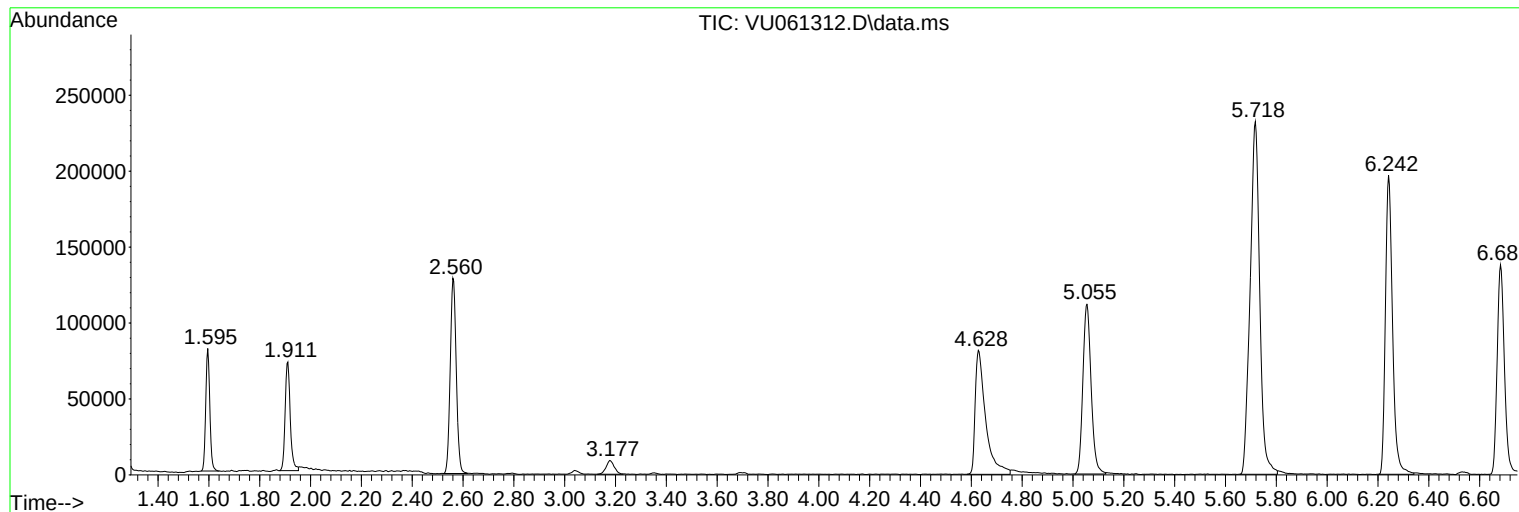

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061312.D
Acq On : 31 Oct 2024 15:26
Operator : MD/SY
Sample : VIBLK152
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061312.D
Acq On : 31 Oct 2024 15:26
Operator : MD/SY
Sample : VIBLK152
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc