

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
 Data File : VU061314.D
 Acq On : 31 Oct 2024 16:15
 Operator : MD/SY
 Sample : VIBLK153
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK153

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rBV	84942	97131	15.31%	1.888%
2	1.911	184	193	211	rBV	76482	104372	16.46%	2.028%
3	2.560	383	395	411	rBV	133308	220847	34.82%	4.292%
4	3.039	535	544	556	rVB3	3378	6394	1.01%	0.124%
5	3.178	574	587	607	rVB	9475	22515	3.55%	0.438%
6	4.628	1023	1038	1076	rBV2	86608	250129	39.44%	4.861%
7	5.055	1154	1171	1198	rBV	117867	262943	41.46%	5.110%
8	5.718	1358	1377	1419	rBV2	240142	634225	100.00%	12.325%
9	6.242	1528	1540	1569	rBV	193053	377249	59.48%	7.331%
10	6.682	1664	1677	1698	rBV	143146	285735	45.05%	5.553%
11	7.560	1939	1950	1971	rBV2	70520	133822	21.10%	2.601%
12	7.891	2040	2053	2074	rBV	298554	542527	85.54%	10.543%
13	8.174	2131	2141	2163	rBV2	40712	76807	12.11%	1.493%
14	8.627	2271	2282	2322	rBV2	281140	588212	92.75%	11.431%
15	9.412	2514	2526	2559	rBV	261856	473661	74.68%	9.205%
16	10.750	2929	2942	2964	rVB	101940	169547	26.73%	3.295%
17	11.804	3259	3270	3295	rBV	256038	433605	68.37%	8.427%
18	12.187	3377	3389	3421	rBV	251533	432317	68.16%	8.402%
19	13.843	3894	3904	3922	rBV3	16699	33660	5.31%	0.654%

Sum of corrected areas: 5145698




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061314.D
Acq On : 31 Oct 2024 16:15
Operator : MD/SY
Sample : VIBLK153
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

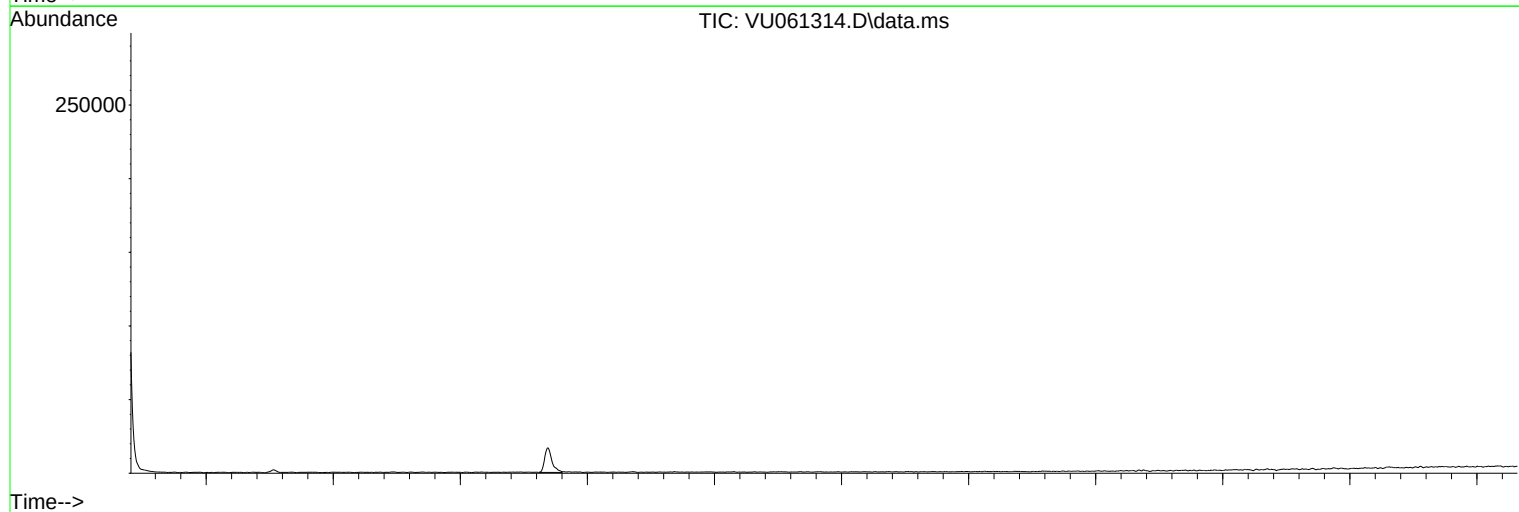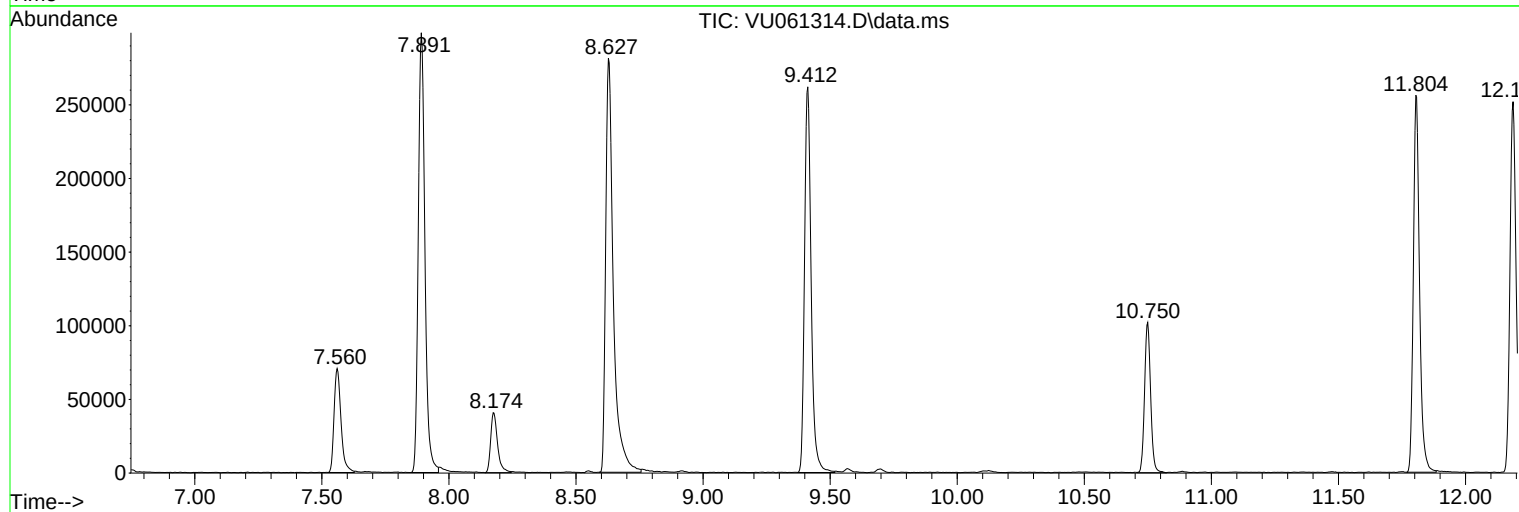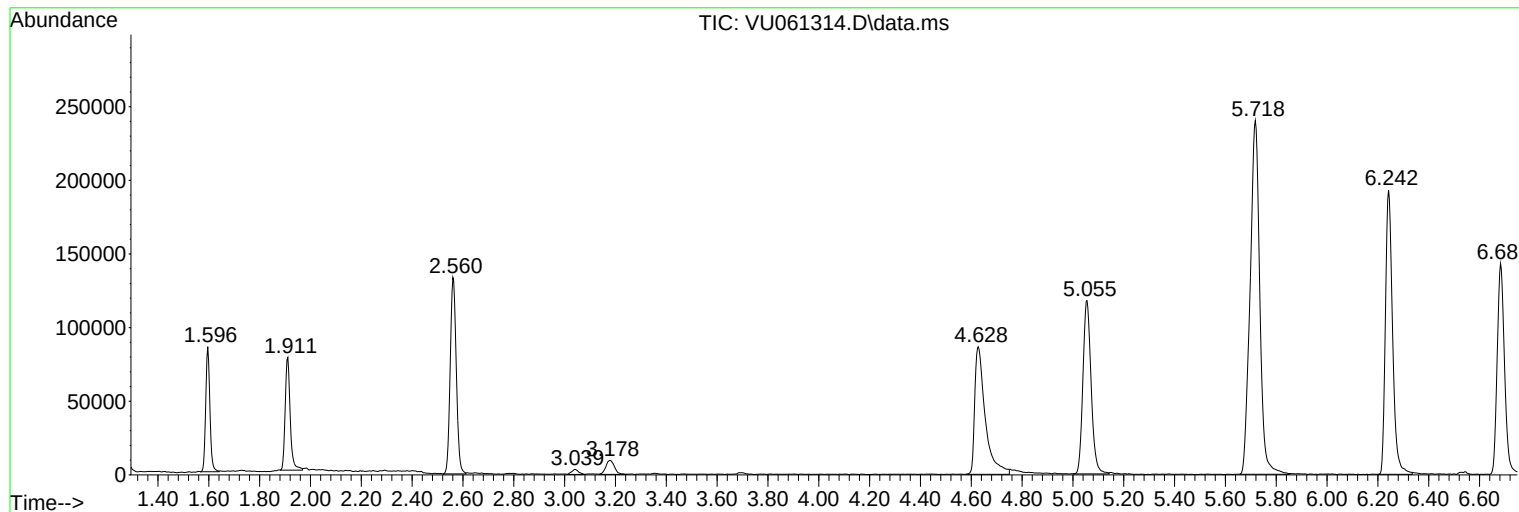

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061314.D
Acq On : 31 Oct 2024 16:15
Operator : MD/SY
Sample : VIBLK153
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103124\
Data File : VU061314.D
Acq On : 31 Oct 2024 16:15
Operator : MD/SY
Sample : VIBLK153
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc