

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110124\  
 Data File : VU061361.D  
 Acq On : 01 Nov 2024 14:37  
 Operator : MD/SY  
 Sample : P4631-19  
 Misc : 25mL/MSVOA\_U/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCP13

Quant Time: Nov 04 04:00:52 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102324WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 01 00:44:02 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)  |
|-------------------------------|--------|-------|----------|----------|-------|-----------|
| -----                         |        |       |          |          |       |           |
| Internal Standards            |        |       |          |          |       |           |
| 1) 1,4-Difluorobenzene        | 6.242  | 114   | 163497   | 5.000    | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 9.412  | 117   | 148886   | 5.000    | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.807 | 152   | 64834    | 5.000    | ug/L  | 0.00      |
|                               |        |       |          |          |       |           |
| System Monitoring Compounds   |        |       |          |          |       |           |
| 4) Vinyl Chloride-d3          | 1.595  | 65    | 40870    | 3.680    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 73.600%   |
| 7) Chloroethane-d5            | 1.907  | 69    | 42311    | 4.156    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 83.200%   |
| 11) 1,1-Dichloroethene-d2     | 2.560  | 65    | 19099    | 4.019    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 80.400%   |
| 20) 2-Butanone-d5             | 4.624  | 46    | 108385   | 48.066   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 96.140%   |
| 24) Chloroform-d              | 5.055  | 84    | 97941    | 4.646    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 93.000%   |
| 26) 1,2-Dichloroethane-d4     | 5.695  | 65    | 51293    | 4.881    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 97.600%   |
| 32) Benzene-d6                | 5.721  | 84    | 196725   | 4.689    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 93.800%   |
| 36) 1,2-Dichloropropane-d6    | 6.682  | 67    | 61436    | 4.871    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 97.400%   |
| 41) Toluene-d8                | 7.891  | 98    | 178666   | 4.555    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 91.000%   |
| 43) trans-1,3-Dichloroprop... | 8.174  | 79    | 21507    | 4.177    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 83.600%   |
| 46) 2-Hexanone-d5             | 8.627  | 63    | 93282    | 44.237   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 88.480%   |
| 56) 1,1,2,2-Tetrachloroeth... | 10.749 | 84    | 45478    | 4.768    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 95.400%   |
| 66) 1,2-Dichlorobenzene-d4    | 12.187 | 152   | 58159    | 5.066    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 101.400%  |
|                               |        |       |          |          |       |           |
| Target Compounds              |        |       |          |          |       |           |
| 13) Acetone                   | 2.644  | 43    | 9190     | 6.435    | ug/L  | Qvalue 96 |
| -----                         |        |       |          |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110124\  
Data File : VU061361.D  
Acq On : 01 Nov 2024 14:37  
Operator : MD/SY  
Sample : P4631-19  
Misc : 25mL/MSVOA\_U/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
GCP13


Quant Time: Nov 04 04:00:52 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR102324WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Nov 01 00:44:02 2024  
Response via : Initial Calibration

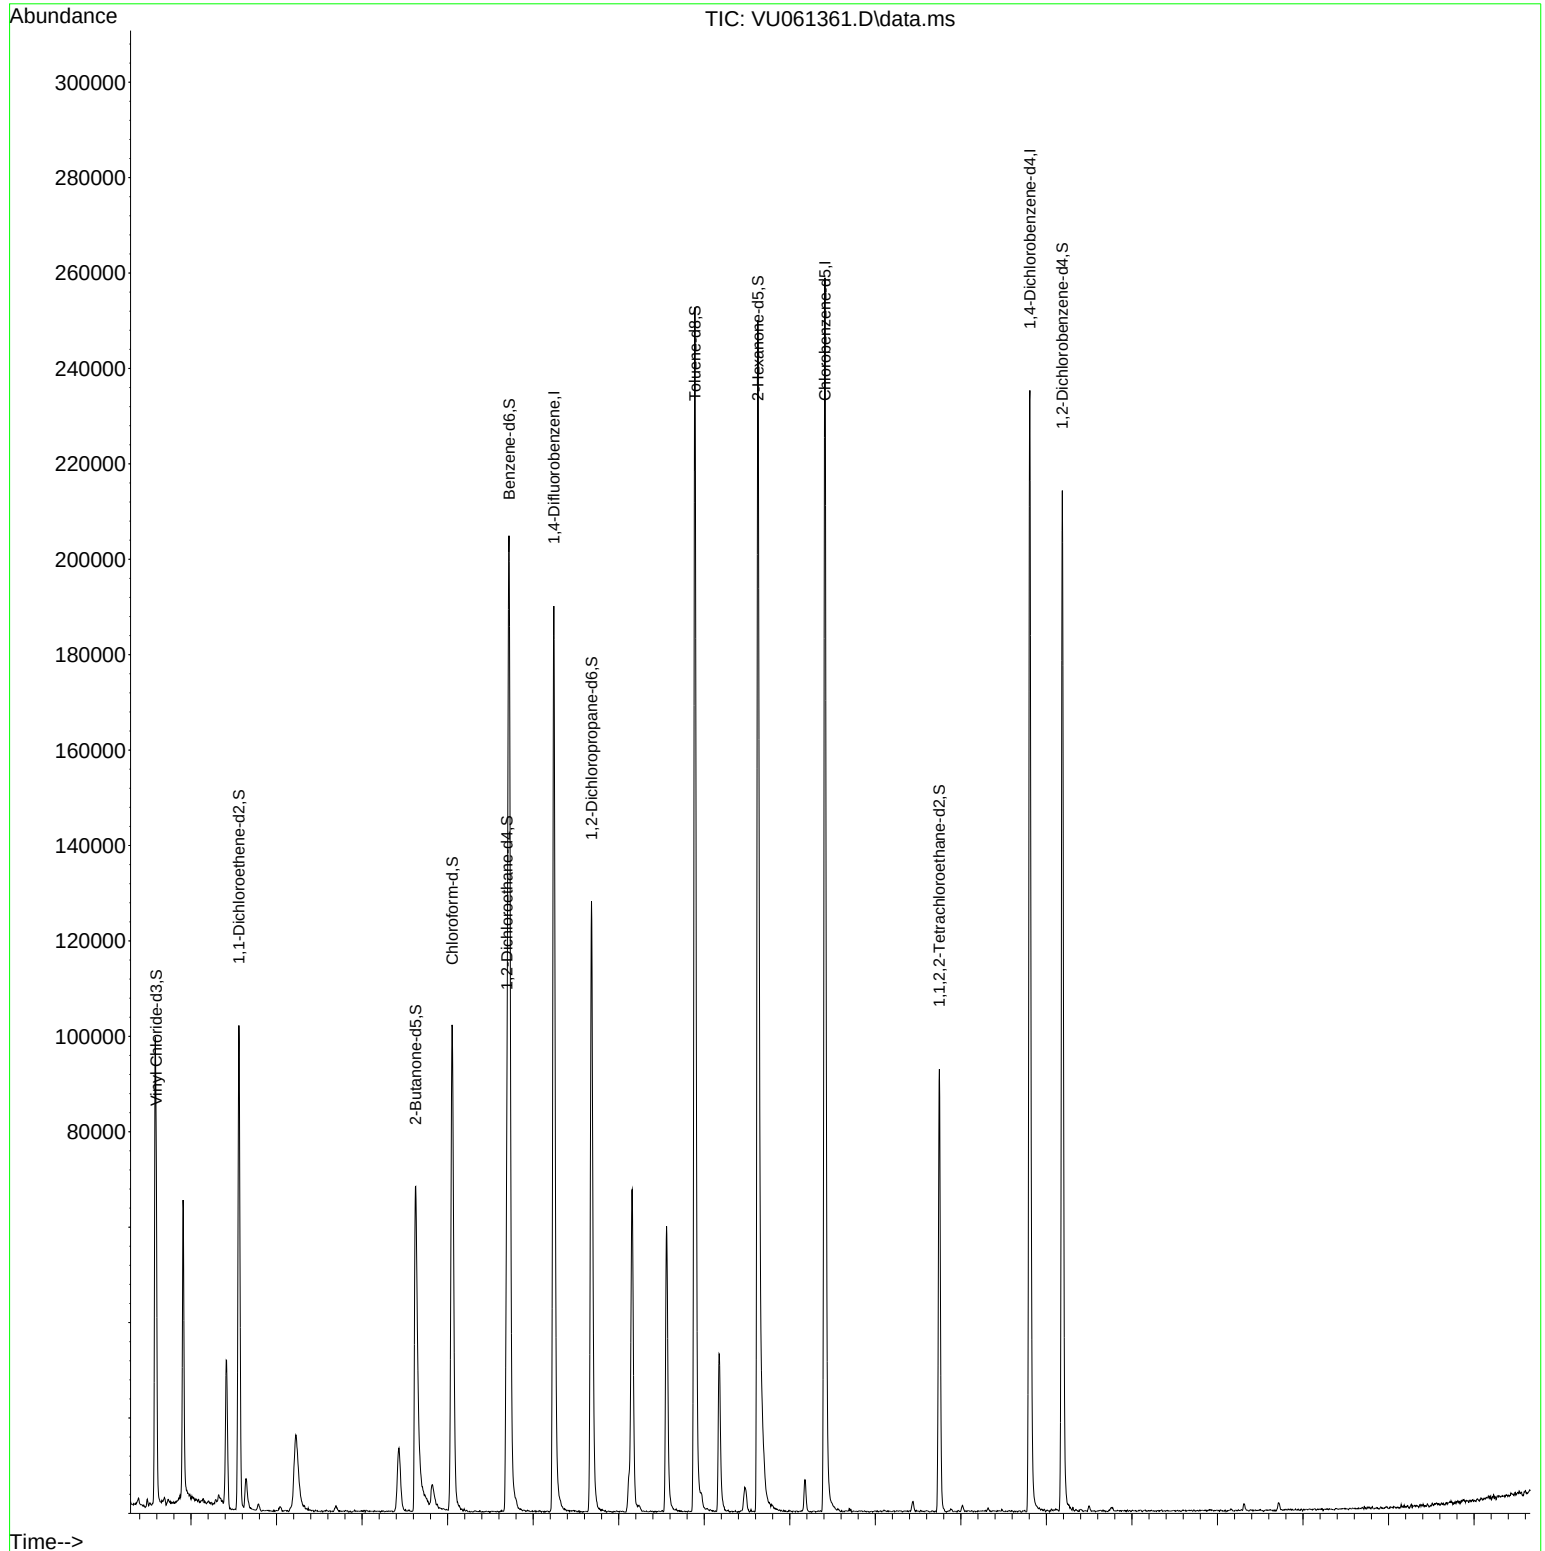

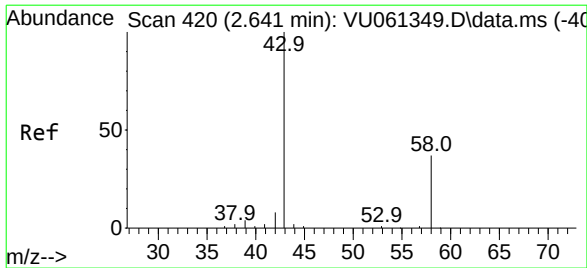

#13  
 Acetone  
 Concen: 6.435 ug/L  
 RT: 2.644 min Scan# 42  
 Delta R.T. -0.000 min  
 Lab File: VU061361.D  
 Acq: 01 Nov 2024 14:37

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 GCP13

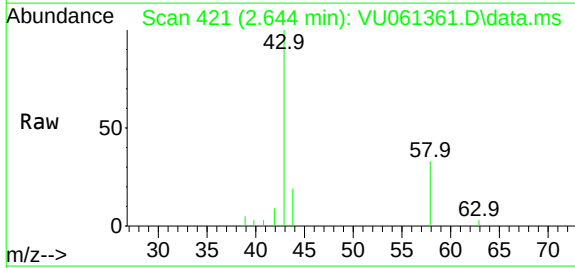

Tgt Ion: 43 Resp: 9190  
 Ion Ratio Lower Upper  
 43 100  
 58 34.3 0.0 73.2

