

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
 Data File : VU061351.D
 Acq On : 01 Nov 2024 10:25
 Operator : MD/SY
 Sample : P4629-10DL 10X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP25DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	110	rBV	62724	72115	12.66%	1.414%
2	1.908	177	192	207	rBV	74134	111189	19.52%	2.179%
3	2.133	254	262	271	rVB2	9048	12704	2.23%	0.249%
4	2.561	382	395	415	rBV	111752	182869	32.10%	3.584%
5	3.181	571	588	603	rBV	10093	22636	3.97%	0.444%
6	4.628	1023	1038	1076	rBV	76224	216875	38.07%	4.251%
7	5.052	1155	1170	1198	rBV	104381	238803	41.92%	4.681%
8	5.718	1356	1377	1407	rBV2	216636	569607	100.00%	11.165%
9	6.242	1527	1540	1574	rBV	195510	386730	67.89%	7.580%
10	6.535	1620	1631	1664	rBV	186476	363268	63.78%	7.120%
11	6.683	1664	1677	1703	rVV	132034	260814	45.79%	5.112%
12	7.560	1936	1950	1976	rBV2	63786	120826	21.21%	2.368%
13	7.891	2040	2053	2086	rBV	270012	492279	86.42%	9.649%
14	8.174	2130	2141	2166	rBV2	36778	67263	11.81%	1.318%
15	8.628	2271	2282	2321	rBV	264253	546746	95.99%	10.717%
16	9.412	2514	2526	2561	rBV	268608	472658	82.98%	9.264%
17	10.750	2929	2942	2959	rBV	95698	156778	27.52%	3.073%
18	11.808	3259	3271	3293	rBV	248425	421330	73.97%	8.258%
19	12.187	3371	3389	3415	rBV	224413	386353	67.83%	7.573%

Sum of corrected areas: 5101843




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061351.D
Acq On : 01 Nov 2024 10:25
Operator : MD/SY
Sample : P4629-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

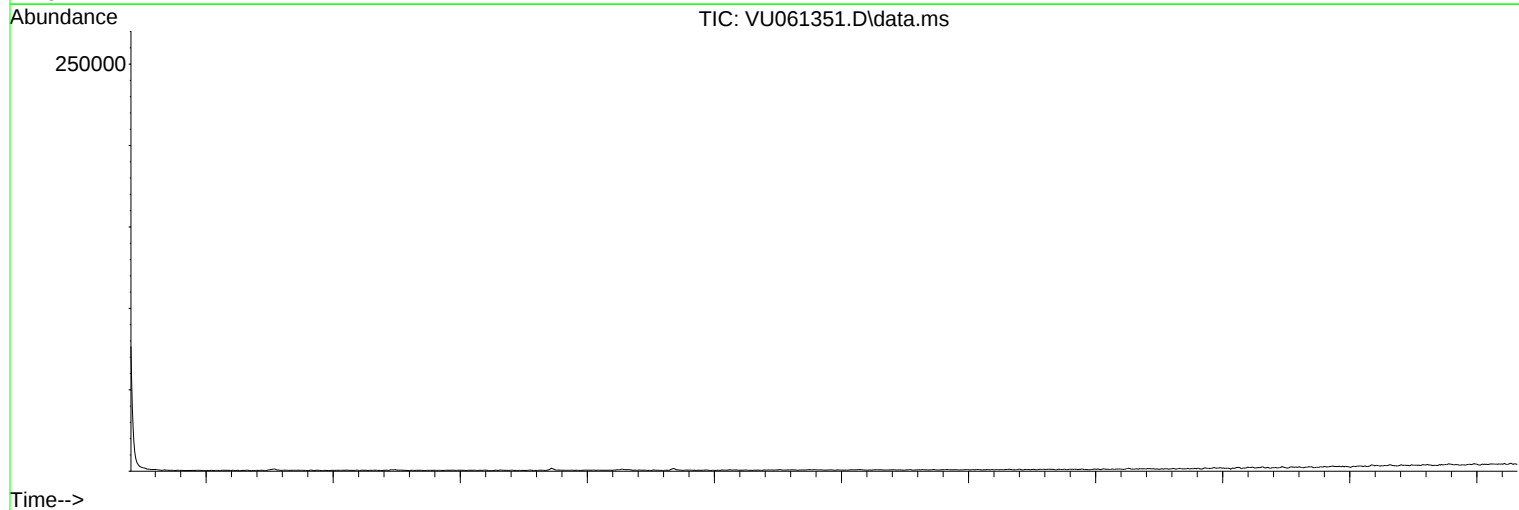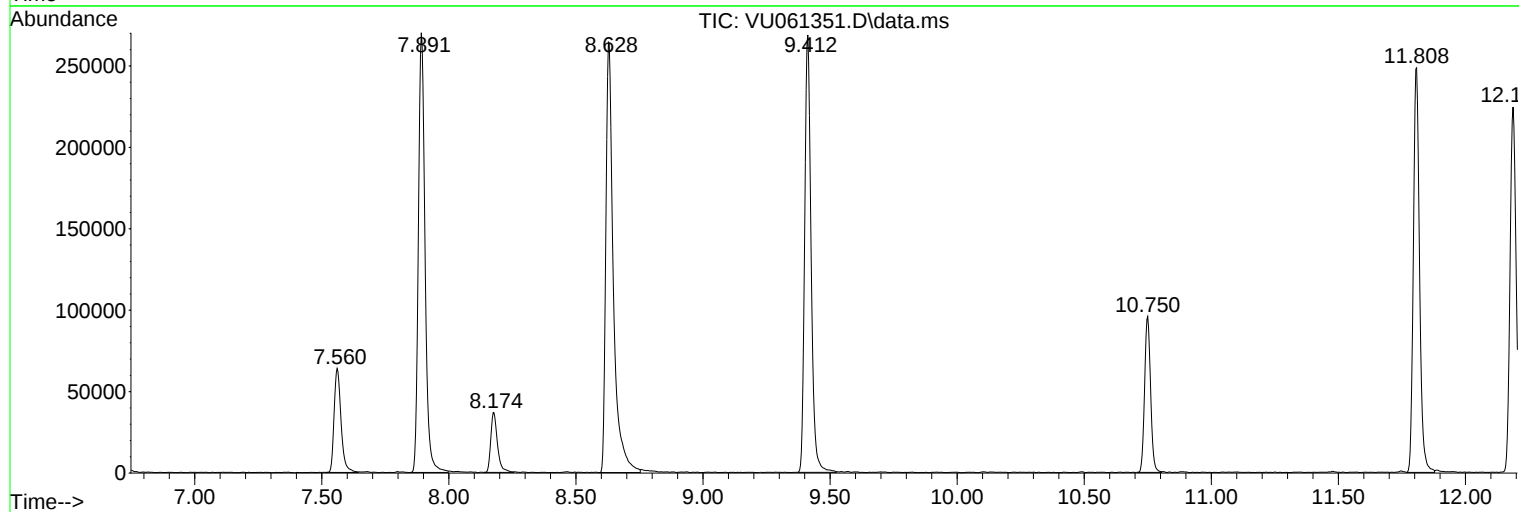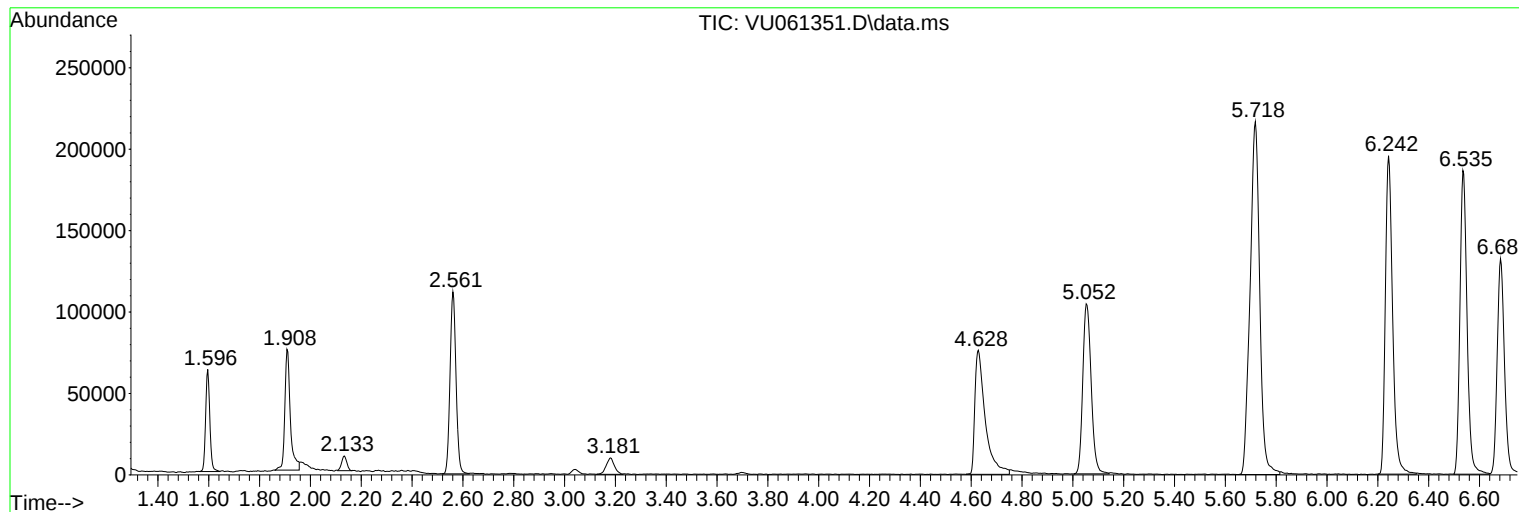

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061351.D
Acq On : 01 Nov 2024 10:25
Operator : MD/SY
Sample : P4629-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061351.D
Acq On : 01 Nov 2024 10:25
Operator : MD/SY
Sample : P4629-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------