

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
 Data File : VU061362.D
 Acq On : 01 Nov 2024 15:02
 Operator : MD/SY
 Sample : P4631-20
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCP14

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	105	rBV	59682	68036	12.97%	1.496%
2	1.907	184	192	206	rBV	63565	82576	15.75%	1.816%
3	2.560	383	395	412	rVB	98965	163431	31.17%	3.594%
4	3.862	788	800	812	rBV2	5415	12844	2.45%	0.282%
5	4.627	1026	1038	1080	rBV2	71465	247348	47.17%	5.439%
6	4.817	1089	1097	1119	rVB3	5783	13785	2.63%	0.303%
7	5.055	1152	1171	1197	rBV	98681	222341	42.40%	4.889%
8	5.717	1358	1377	1411	rBV2	201906	524384	100.00%	11.532%
9	6.242	1527	1540	1572	rBV	197064	382635	72.97%	8.414%
10	6.537	1621	1632	1652	rVB2	27361	52386	9.99%	1.152%
11	6.682	1664	1677	1700	rBV	122891	244791	46.68%	5.383%
12	7.560	1936	1950	1975	rBV2	57439	107485	20.50%	2.364%
13	7.891	2035	2053	2091	rBV	245689	445951	85.04%	9.807%
14	8.177	2132	2142	2165	rBV	33090	60940	11.62%	1.340%
15	8.550	2249	2258	2267	rBV3	5878	9159	1.75%	0.201%
16	8.627	2272	2282	2314	rBV2	249239	514296	98.08%	11.310%
17	9.412	2514	2526	2555	rBV	270572	473779	90.35%	10.419%
18	10.749	2929	2942	2964	rBV	89490	148115	28.25%	3.257%
19	11.807	3259	3271	3297	rBV	246926	416908	79.50%	9.168%
20	12.187	3375	3389	3419	rBV	204378	356200	67.93%	7.833%

Sum of corrected areas: 4547390




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061362.D
Acq On : 01 Nov 2024 15:02
Operator : MD/SY
Sample : P4631-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

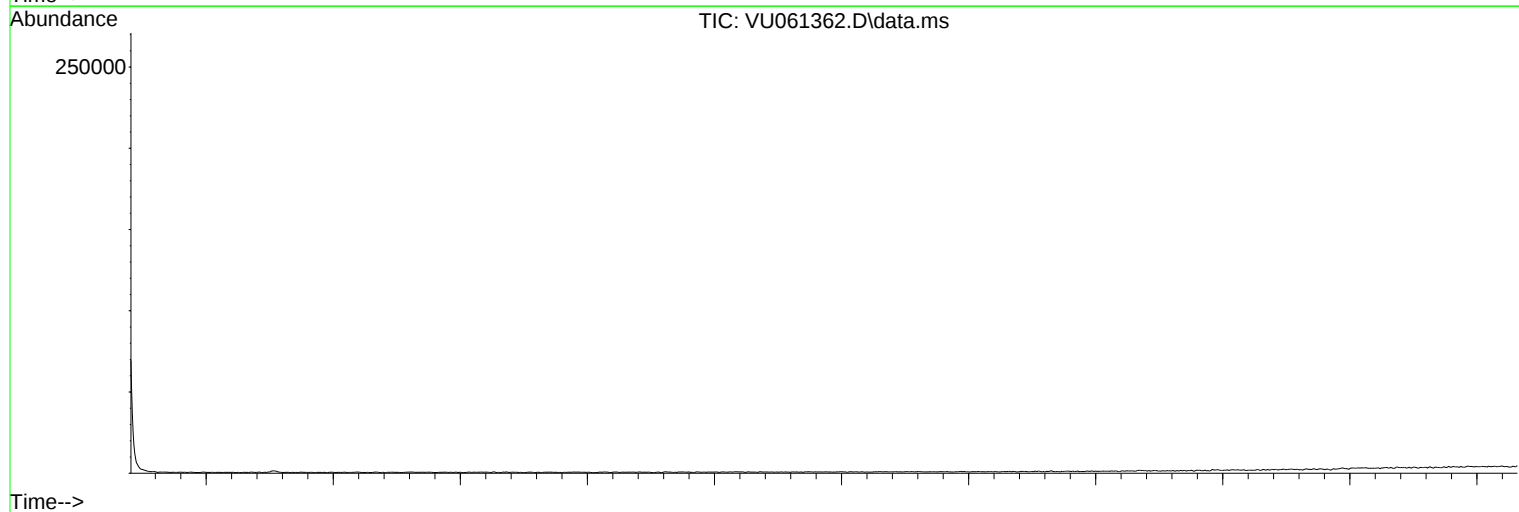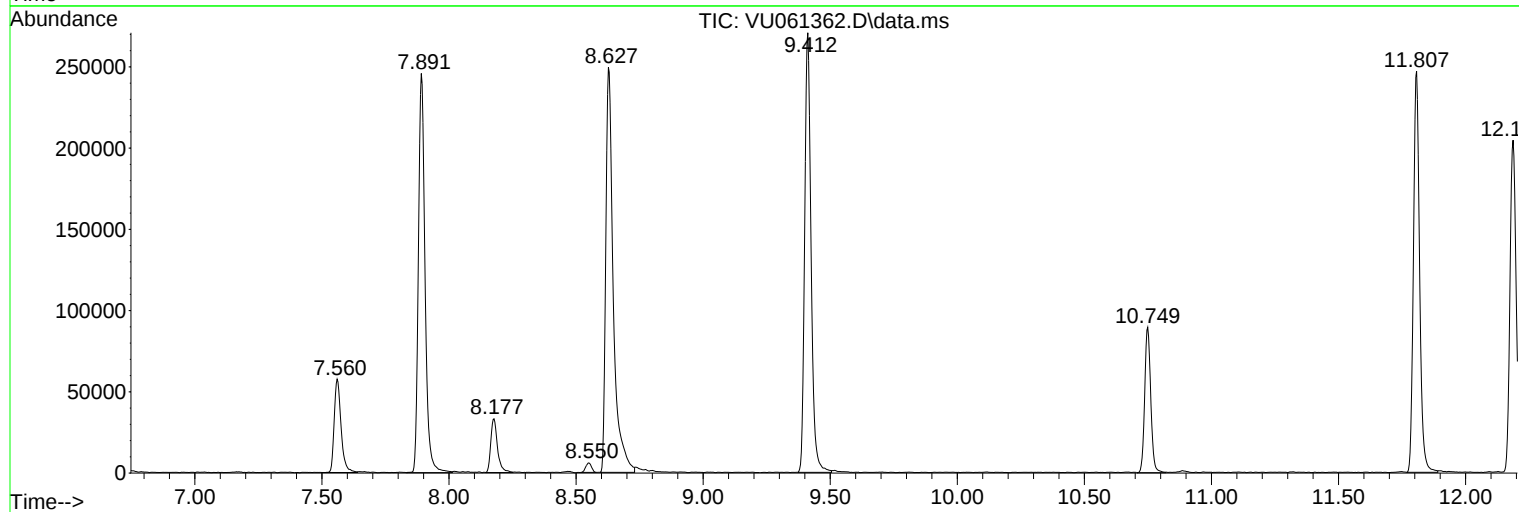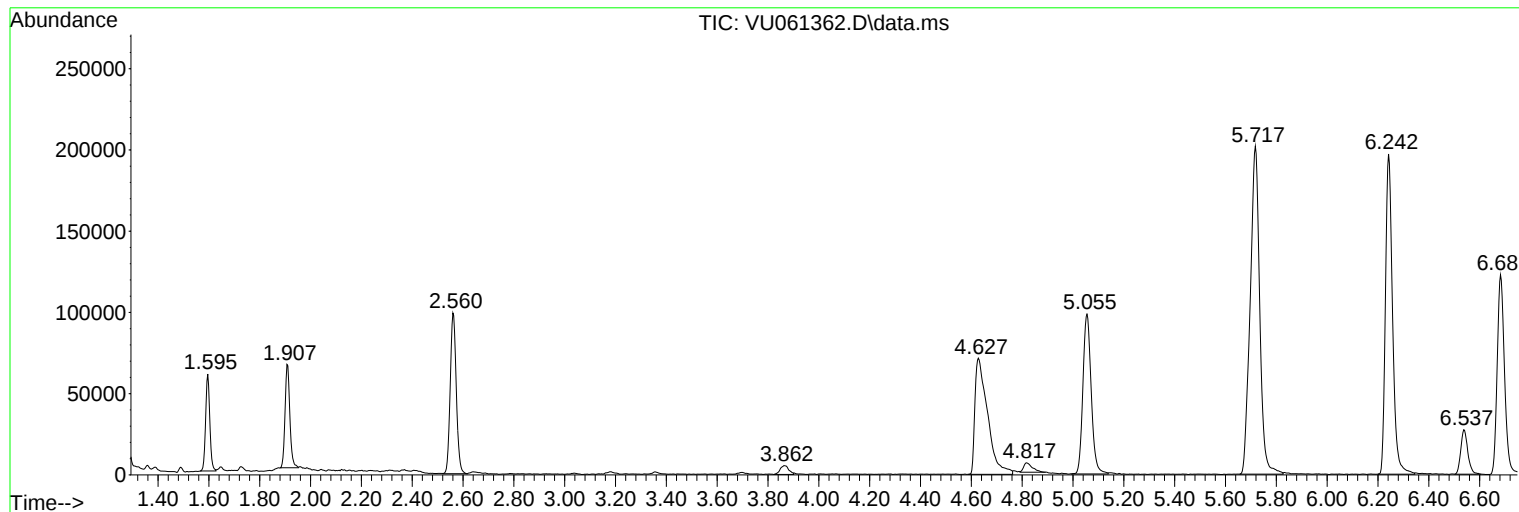

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061362.D
Acq On : 01 Nov 2024 15:02
Operator : MD/SY
Sample : P4631-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061362.D
Acq On : 01 Nov 2024 15:02
Operator : MD/SY
Sample : P4631-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCP14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc