

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
 Data File : VU061371.D
 Acq On : 01 Nov 2024 18:43
 Operator : MD/SY
 Sample : P4625-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	85	95	105	rVB	54033	64387	12.50%	1.428%
2	1.840	157	171	173	rBV7	3576	6747	1.31%	0.150%
3	1.907	184	192	206	rVB	51702	69499	13.49%	1.541%
4	2.560	383	395	412	rBV	94761	153416	29.78%	3.402%
5	3.862	790	800	818	rVB	3829	9059	1.76%	0.201%
6	4.621	1023	1036	1061	rBV	71692	185584	36.02%	4.116%
7	5.052	1156	1170	1196	rBV	95323	216968	42.11%	4.811%
8	5.717	1359	1377	1407	rBV2	194946	512184	99.41%	11.358%
9	6.241	1526	1540	1571	rBV	188485	373482	72.49%	8.282%
10	6.682	1664	1677	1701	rBV	119279	237399	46.08%	5.265%
11	7.560	1939	1950	1970	rBV	57390	103998	20.19%	2.306%
12	7.891	2041	2053	2066	rBV	235971	418646	81.26%	9.284%
13	7.962	2066	2075	2095	rVB	108144	197962	38.42%	4.390%
14	8.174	2129	2141	2159	rBV2	32672	58532	11.36%	1.298%
15	8.627	2271	2282	2327	rBV2	251623	515217	100.00%	11.425%
16	9.412	2514	2526	2550	rBV	258878	455780	88.46%	10.107%
17	10.749	2930	2942	2963	rBV	89600	145445	28.23%	3.225%
18	11.804	3259	3270	3294	rBV	235916	402633	78.15%	8.929%
19	12.187	3376	3389	3413	rBV	201381	347579	67.46%	7.708%
20	17.280	4963	4973	4983	rBV2	23946	34866	6.77%	0.773%




Sum of corrected areas: 4509383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061371.D
Acq On : 01 Nov 2024 18:43
Operator : MD/SY
Sample : P4625-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

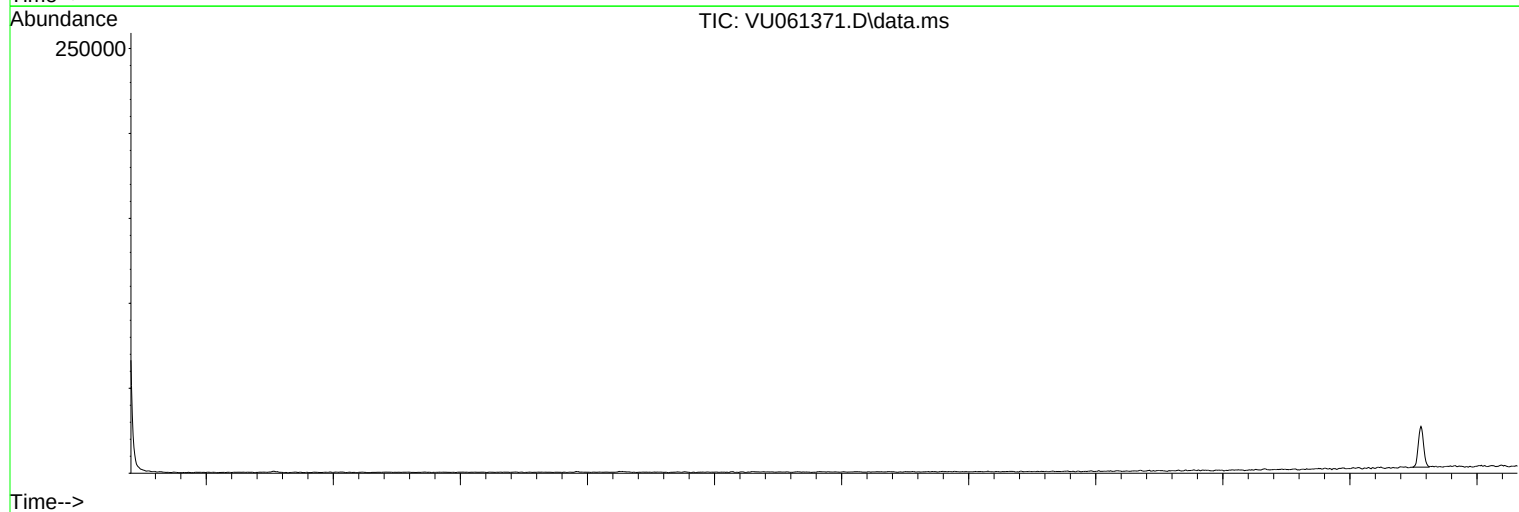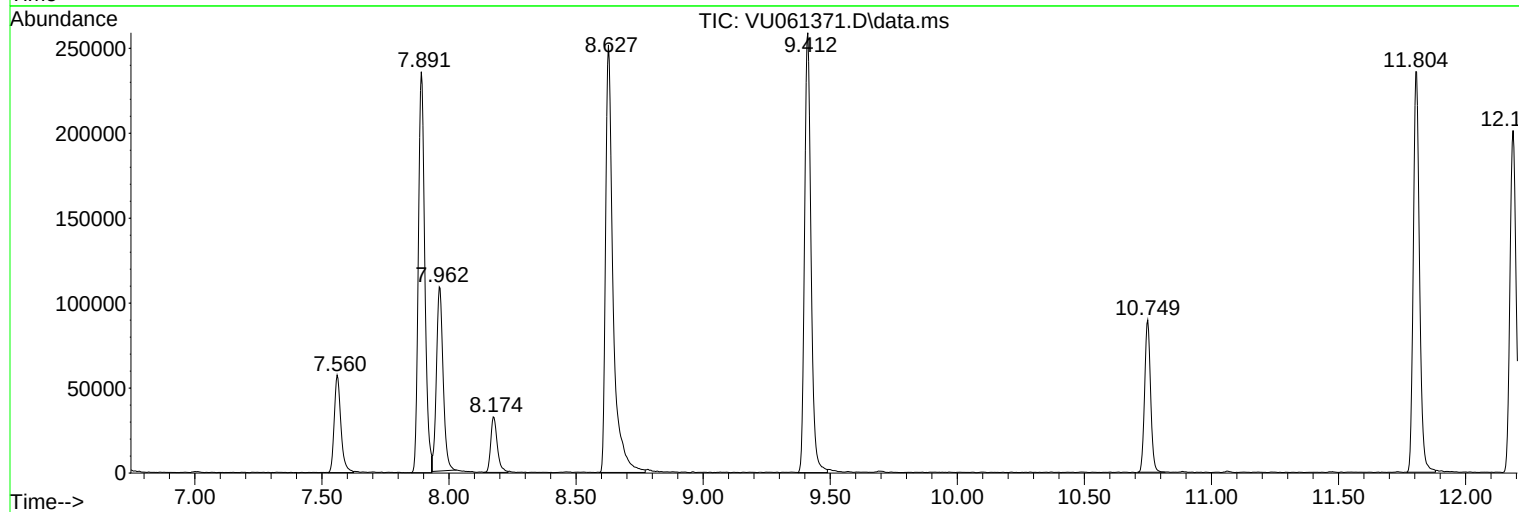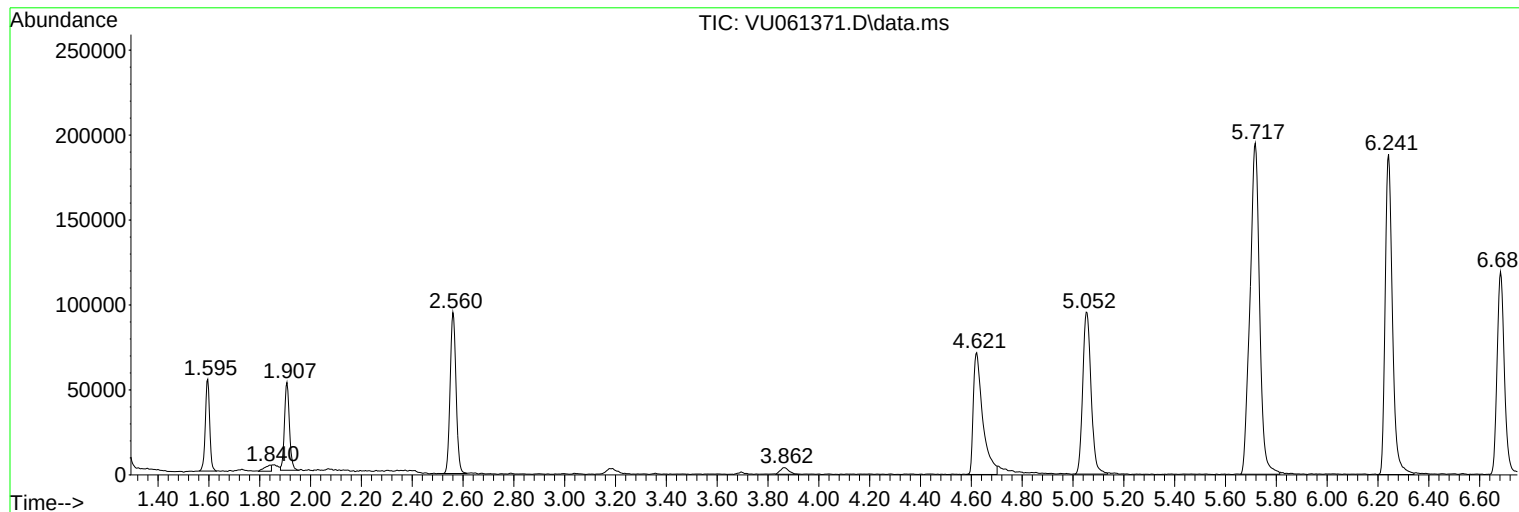

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061371.D
Acq On : 01 Nov 2024 18:43
Operator : MD/SY
Sample : P4625-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061371.D
Acq On : 01 Nov 2024 18:43
Operator : MD/SY
Sample : P4625-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc