

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
 Data File : VU061378.D
 Acq On : 01 Nov 2024 22:24
 Operator : MD/SY
 Sample : P4625-13
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	108	rVB	56099	65388	4.84%	1.097%
2	1.908	184	192	207	rVB	63541	86377	6.39%	1.449%
3	2.560	384	395	411	rBV	96578	157736	11.67%	2.647%
4	4.621	1026	1036	1078	rBV	69315	191824	14.19%	3.219%
5	5.052	1156	1170	1193	rBV	95844	218328	16.15%	3.663%
6	5.718	1356	1377	1404	rBV2	197640	521980	38.62%	8.758%
7	6.242	1526	1540	1561	rBV	198542	386391	28.59%	6.483%
8	6.682	1663	1677	1698	rBV	121854	242432	17.94%	4.068%
9	7.560	1939	1950	1973	rBV	57828	106613	7.89%	1.789%
10	7.891	2041	2053	2064	rBV	250442	435683	32.23%	7.310%
11	7.962	2064	2075	2110	rVB	756670	1351608	100.00%	22.679%
12	8.177	2131	2142	2161	rVB	31273	56423	4.17%	0.947%
13	8.627	2270	2282	2321	rBV2	261699	540296	39.97%	9.066%
14	9.409	2513	2525	2550	rBV	270405	474009	35.07%	7.953%
15	10.746	2927	2941	2959	rBV	90342	150807	11.16%	2.530%
16	11.804	3259	3270	3292	rBV	257180	424381	31.40%	7.121%
17	12.087	3347	3358	3373	rBV	38337	61085	4.52%	1.025%
18	12.187	3377	3389	3411	rBV	213325	360155	26.65%	6.043%
19	14.084	3968	3979	3999	rBV	57862	104324	7.72%	1.750%
20	17.280	4965	4973	4984	rBV2	15794	23957	1.77%	0.402%




Sum of corrected areas: 5959797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061378.D
Acq On : 01 Nov 2024 22:24
Operator : MD/SY
Sample : P4625-13
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

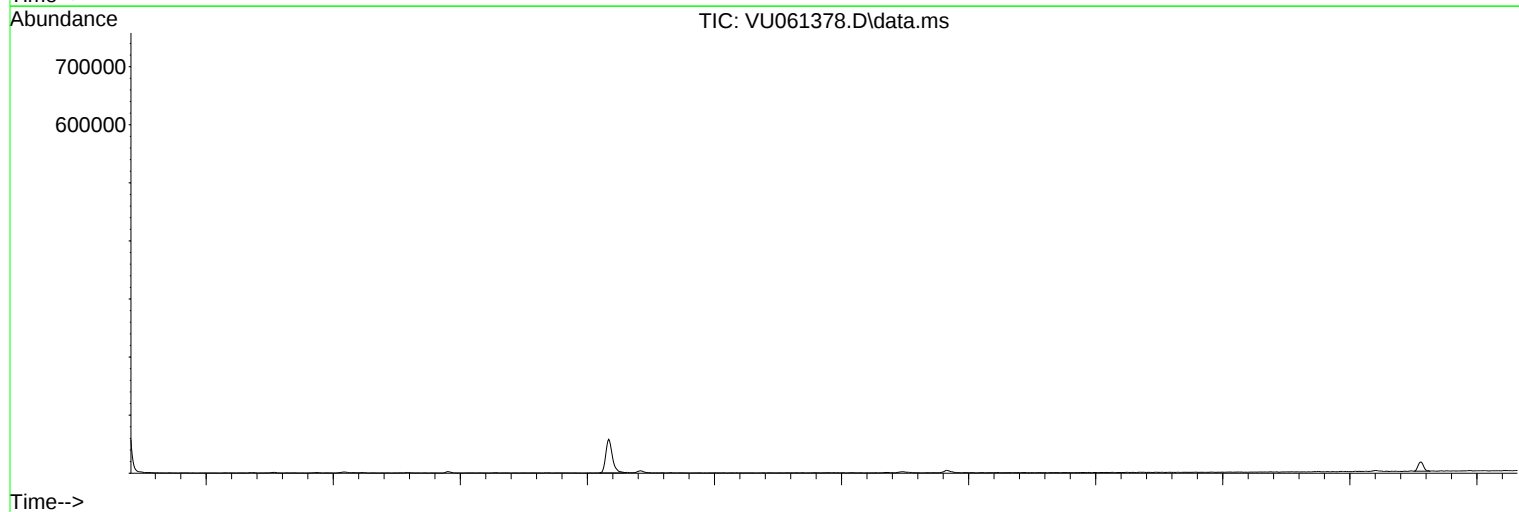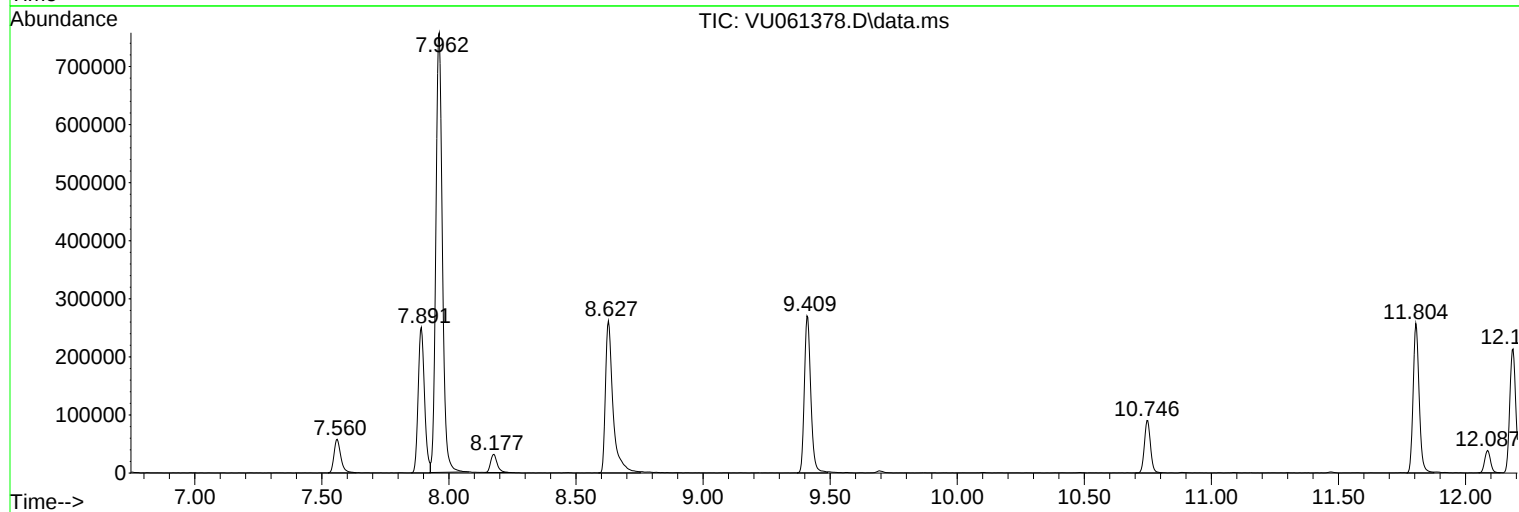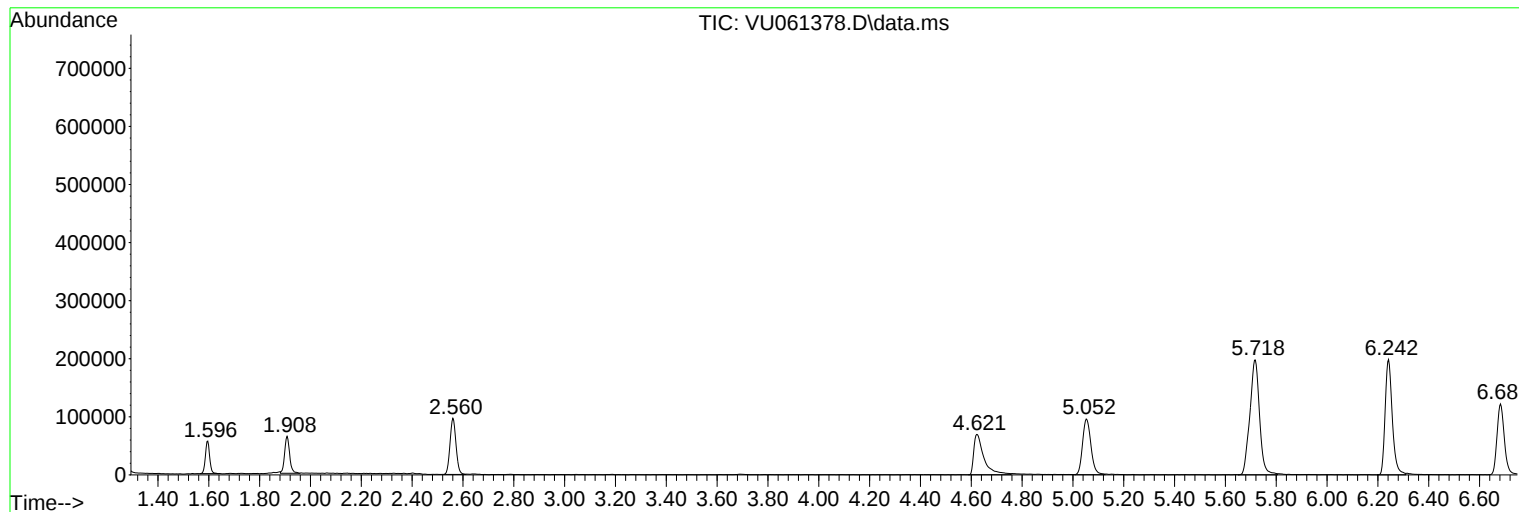

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061378.D
Acq On : 01 Nov 2024 22:24
Operator : MD/SY
Sample : P4625-13
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.087	0.72 ug/L	61085	1,4-Dichlorobenzene-d4	11.804

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane	118	C9H10	000496-11-7	90
2	1,3-Methanopentalene, 1,2,3,5-te...	118	C9H10	128600-88-4	64
3	Tetracyclo[3.3.1.0(2,8).0(4,6)]-...	118	C9H10	1000191-13-7	64
4	Indane	118	C9H10	000496-11-7	60
5	Indane	118	C9H10	000496-11-7	55

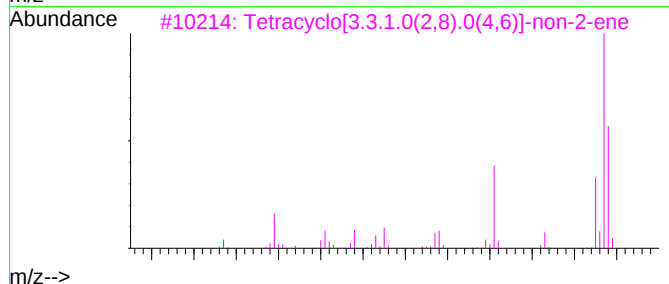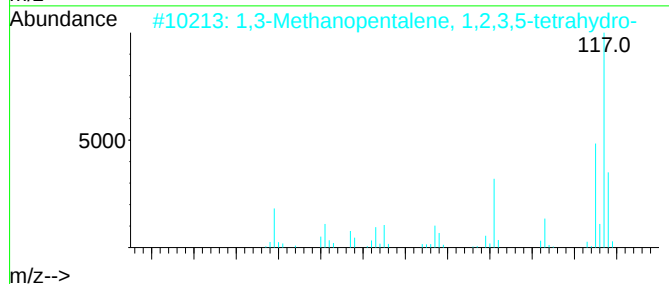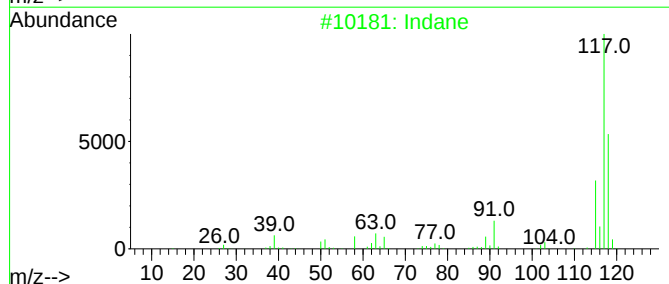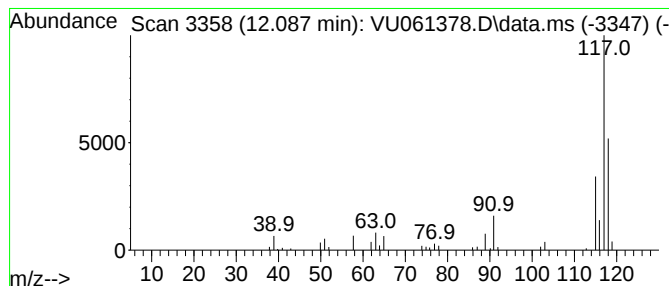

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061378.D
Acq On : 01 Nov 2024 22:24
Operator : MD/SY
Sample : P4625-13
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 1H-Indene, 1-methylene- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.084	1.23 ug/L	104324	1,4-Dichlorobenzene-d4	11.804

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Naphthalene	128	C10H8	000091-20-3	95
2	1H-Indene, 1-methylene-	128	C10H8	002471-84-3	95
3	Naphthalene	128	C10H8	000091-20-3	93
4	Azulene	128	C10H8	000275-51-4	91
5	Naphthalene	128	C10H8	000091-20-3	91

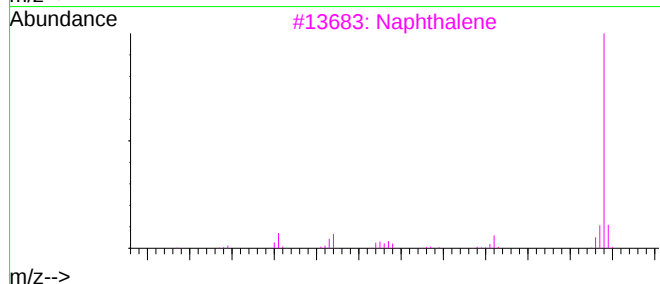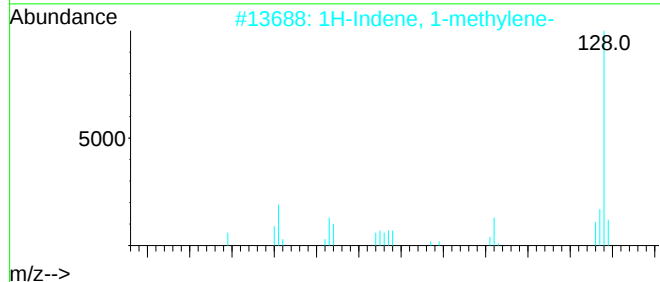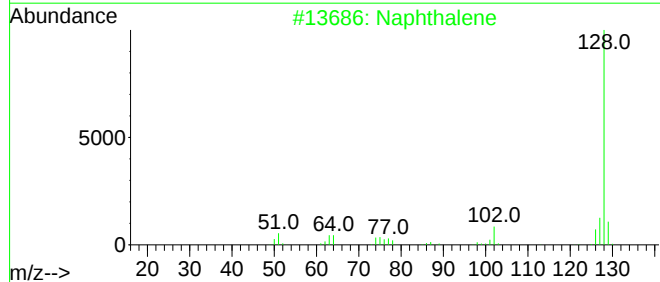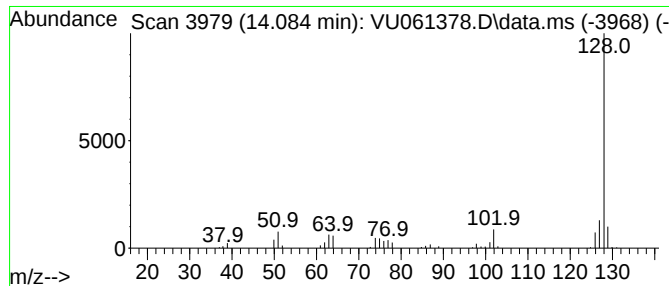

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061378.D
Acq On : 01 Nov 2024 22:24
Operator : MD/SY
Sample : P4625-13
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.087	0.7	ug/L	61085	3	11.804	424381	5.0
1H-Indene, 1-me...	14.084	1.2	ug/L	104324	3	11.804	424381	5.0