

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
 Data File : VU061379.D
 Acq On : 01 Nov 2024 22:49
 Operator : MD/SY
 Sample : P4625-14
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AC2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	110	rBV	54243	65777	12.95%	1.517%
2	1.907	183	192	205	rVB	56561	75987	14.96%	1.752%
3	2.560	383	395	412	rBV	92596	151604	29.85%	3.495%
4	4.621	1027	1036	1075	rBV	65083	178702	35.19%	4.120%
5	5.055	1155	1171	1196	rBV	94144	212571	41.85%	4.901%
6	5.718	1358	1377	1404	rBV2	190947	502393	98.92%	11.583%
7	6.242	1528	1540	1570	rBV	190974	374341	73.70%	8.631%
8	6.682	1664	1677	1702	rBV	116864	232743	45.83%	5.366%
9	7.560	1939	1950	1974	rBV	53721	102947	20.27%	2.374%
10	7.891	2039	2053	2070	rBV	235226	419188	82.54%	9.665%
11	7.968	2070	2077	2089	rVB2	12335	22492	4.43%	0.519%
12	8.174	2132	2141	2169	rBV	30639	55650	10.96%	1.283%
13	8.627	2268	2282	2329	rBV2	243318	507891	100.00%	11.710%
14	9.412	2513	2526	2557	rBV	259891	458565	90.29%	10.572%
15	9.692	2604	2613	2626	rVB2	3657	6506	1.28%	0.150%
16	10.746	2931	2941	2961	rBV	87198	143801	28.31%	3.315%
17	11.804	3259	3270	3295	rBV	241414	404050	79.55%	9.316%
18	12.087	3348	3358	3373	rBV	22042	33143	6.53%	0.764%
19	12.187	3376	3389	3410	rBV	203881	340362	67.01%	7.847%
20	14.087	3970	3980	4004	rBV2	23961	48626	9.57%	1.121%




Sum of corrected areas: 4337339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061379.D
Acq On : 01 Nov 2024 22:49
Operator : MD/SY
Sample : P4625-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

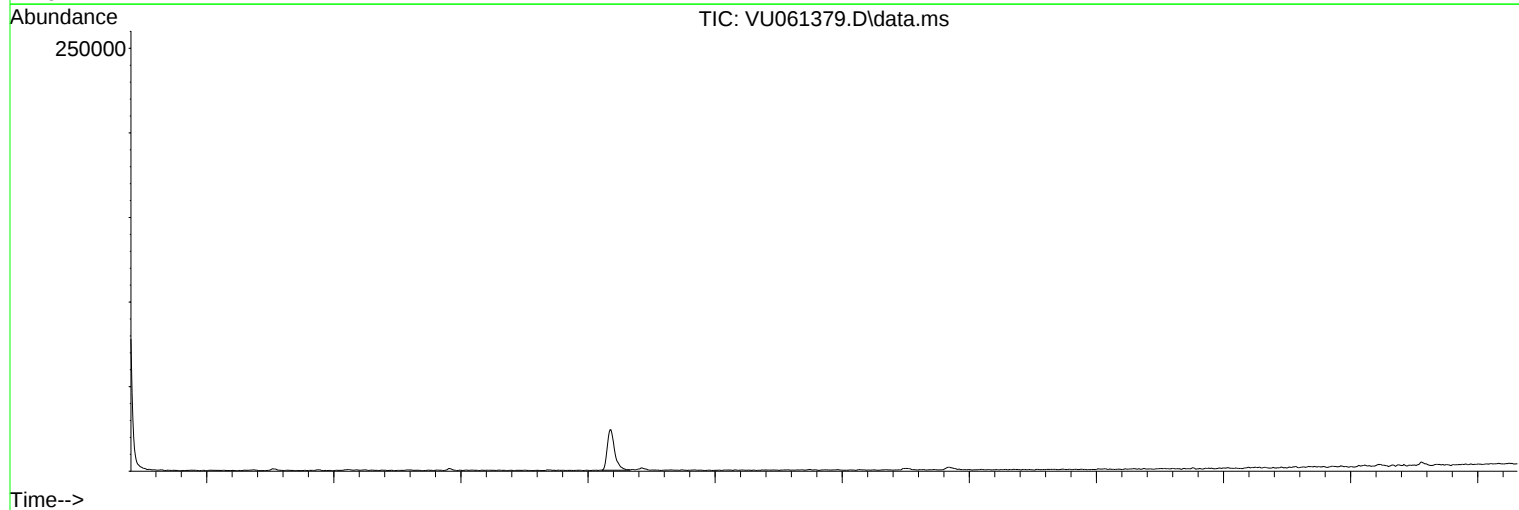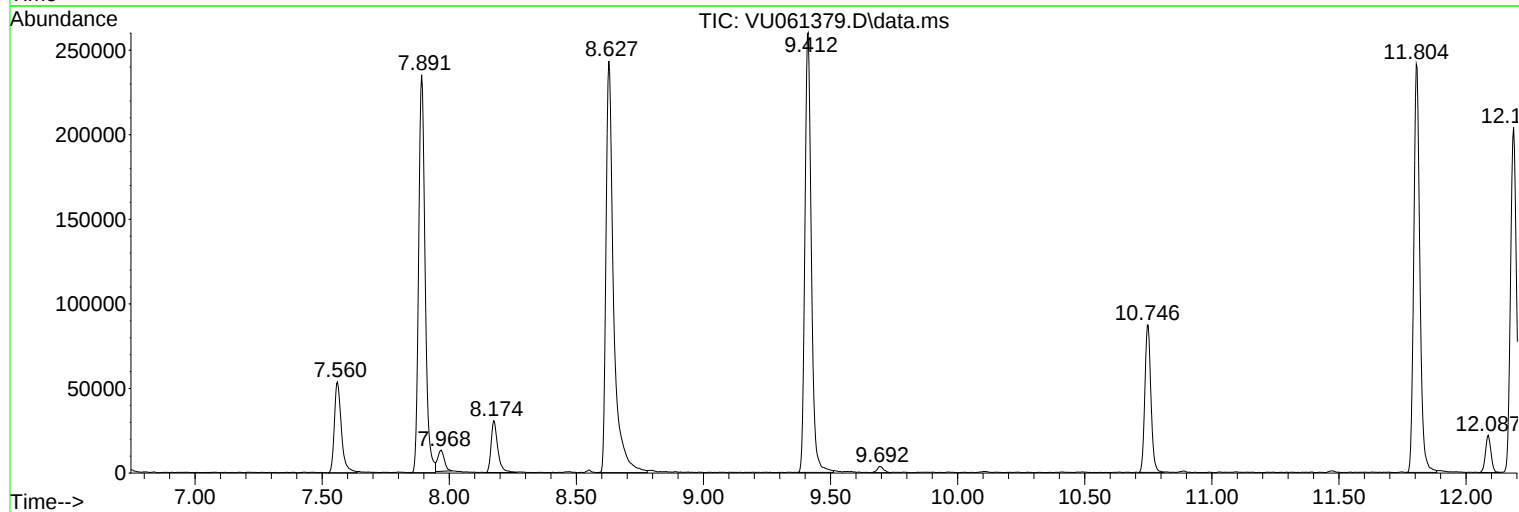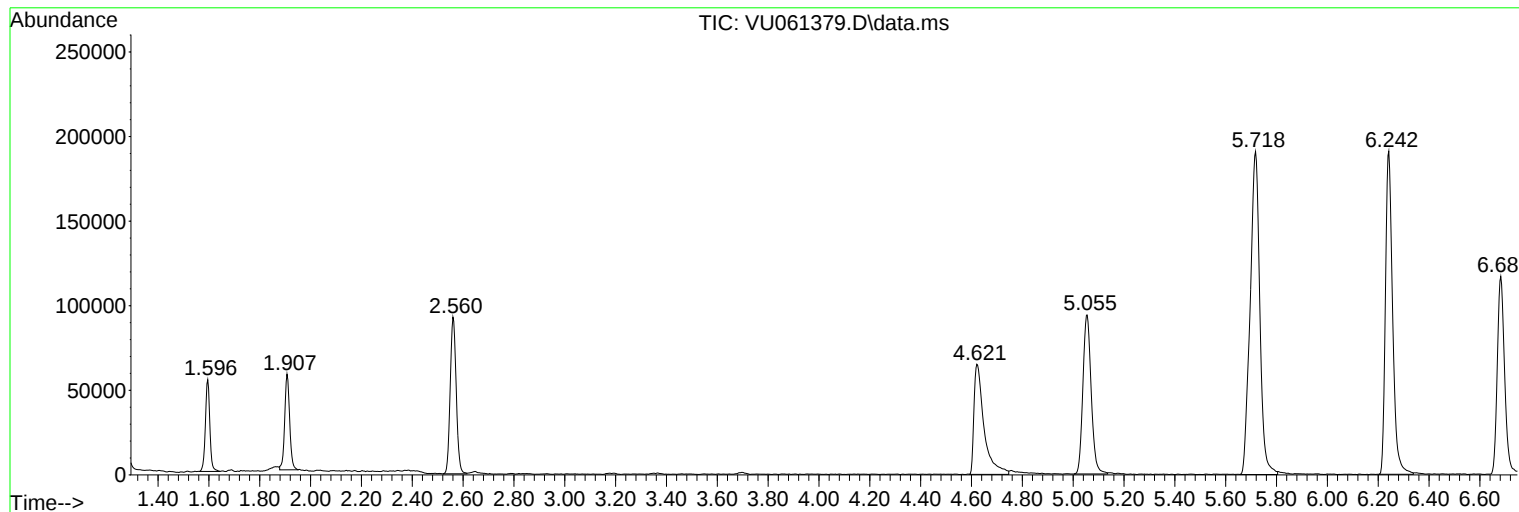

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061379.D
Acq On : 01 Nov 2024 22:49
Operator : MD/SY
Sample : P4625-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1










Instrument :
MSVOA_U
ClientSampleId :
C0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Indene, 1-methylene- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD		R.T.	
14.087	0.60 ug/L	48626	1,4-Dichlorobenzene-d4		11.804	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Naphthalene		128	C10H8	000091-20-3	95
2	1H-Indene, 1-methylene-		128	C10H8	002471-84-3	95
3	Azulene		128	C10H8	000275-51-4	91
4	Azulene		128	C10H8	000275-51-4	91
5	Naphthalene		128	C10H8	000091-20-3	91

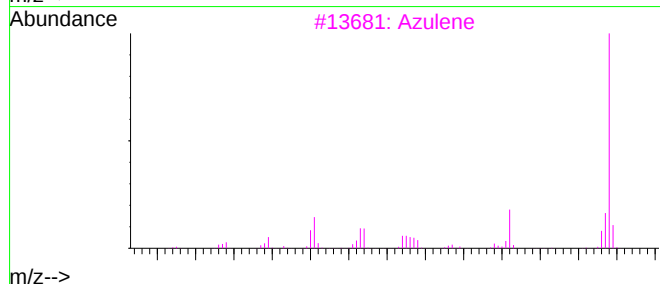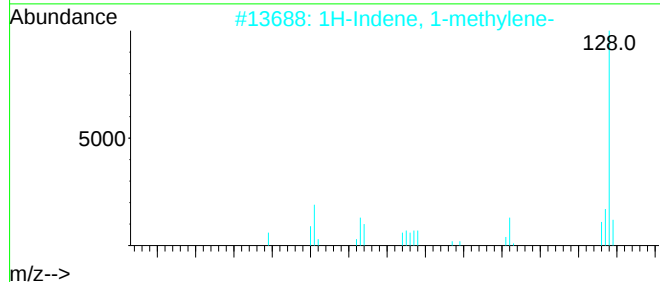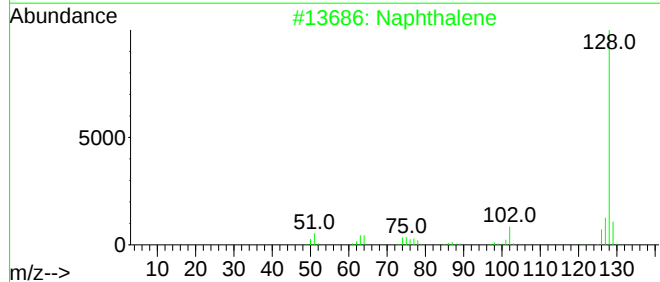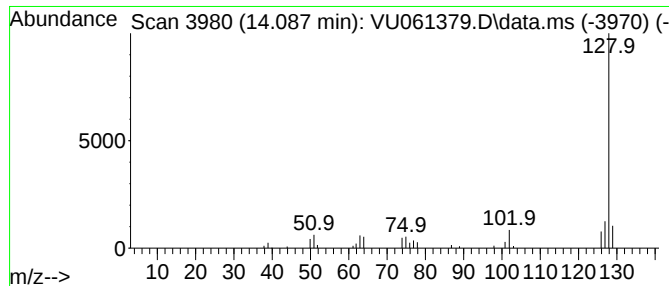

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061379.D
Acq On : 01 Nov 2024 22:49
Operator : MD/SY
Sample : P4625-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 1-me...	14.087	0.6	ug/L	48626	3	11.804	404050	5.0