
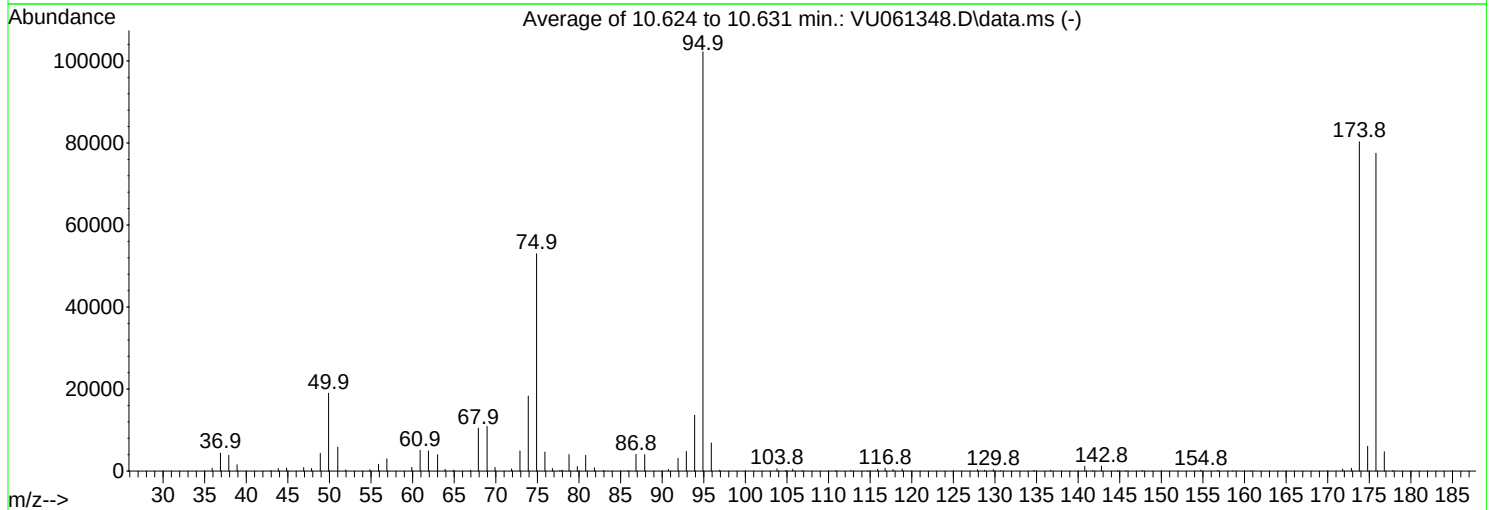


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110124\
Data File : VU061348.D
Acq On : 01 Nov 2024 08:27
Operator : MD/SY
Sample : BFB018
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB018

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 05 04:38:45 2024

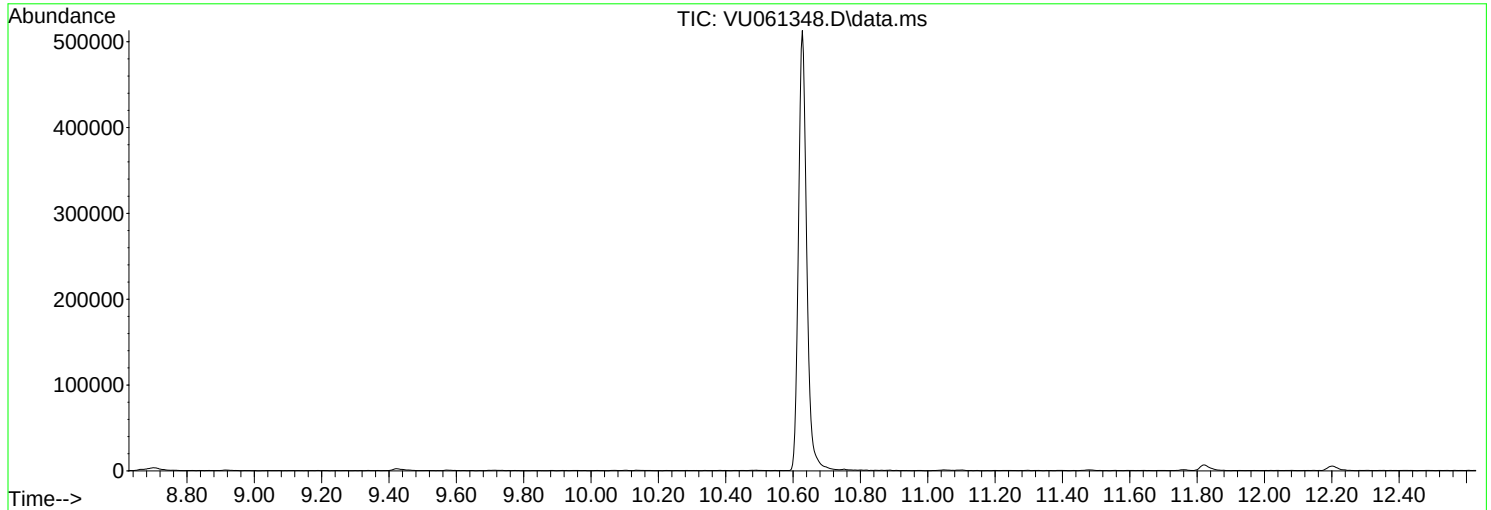

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	18976	PASS
75	95	30	80	51.8	52997	PASS
95	95	100	100	100.0	102251	PASS
96	95	5	9	6.7	6872	PASS
173	174	0.00	2	0.8	664	PASS
174	95	50	120	78.5	80309	PASS
175	174	5	9	7.5	6024	PASS
176	174	95	101	96.5	77493	PASS
177	176	5	9	6.1	4723	PASS

Scan 2890 (10.582 min): VU061348.D\data.ms
BFB018

m/z	Abundance
39.90	151.0
43.80	294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	698.0
36.90	4390.0
37.90	3936.0
38.90	1495.0
39.90	128.0
42.90	144.0
43.90	974.0
44.90	791.0
46.90	966.0
47.80	673.0
48.90	4386.0
49.90	19144.0
51.00	5664.0
51.90	293.0
54.80	334.0
55.90	1625.0
56.90	2819.0
59.90	917.0
60.90	5141.0
61.90	4946.0
63.00	4029.0
63.90	487.0
64.90	226.0
67.00	191.0
67.90	10480.0
68.90	10839.0
69.90	909.0
71.90	529.0
72.90	4789.0
73.90	18360.0
74.90	53032.0
75.90	4622.0
76.80	668.0
77.90	367.0
78.80	4064.0
79.80	1077.0
80.80	3740.0
81.80	788.0
83.00	131.0
85.90	136.0
86.80	4072.0
87.90	4060.0
90.80	439.0
91.90	3140.0
92.90	4857.0
93.90	13395.0
94.90	101752.0
95.90	7212.0
96.90	200.0
103.80	618.0
104.80	150.0
105.70	493.0
106.80	124.0
110.90	130.0
112.70	115.0
115.90	400.0
116.80	711.0
117.70	363.0
118.90	545.0
127.90	379.0
128.70	197.0
129.80	385.0
130.70	130.0
134.70	189.0
136.70	208.0
140.80	1110.0
141.70	131.0
142.80	1148.0
144.80	161.0
145.70	137.0
147.70	200.0
154.70	232.0
156.80	210.0
158.60	111.0
160.70	105.0
171.80	452.0
172.90	624.0
173.80	77568.0
174.80	5996.0
175.80	75120.0
176.80	4793.0
177.80	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	725.0
36.90	4562.0
37.90	3930.0
38.90	1601.0
40.00	117.0
42.90	119.0
43.90	935.0
44.90	784.0
46.90	906.0
47.90	658.0
48.90	4503.0
49.90	19536.0
51.00	6096.0
52.00	294.0
54.90	333.0
55.90	1709.0
56.90	3091.0
59.90	986.0
60.90	5191.0
61.90	5074.0
63.00	4103.0
63.90	453.0
64.90	221.0
66.90	220.0
67.90	10793.0
69.00	11260.0
69.90	961.0
71.90	556.0
72.90	5076.0
73.90	18872.0
74.90	54504.0
75.90	4768.0
76.80	654.0
78.00	358.0
78.80	4204.0
79.80	1130.0
80.80	3936.0
81.80	849.0
82.90	132.0
85.90	124.0
86.90	4148.0
87.90	4179.0
90.80	424.0
91.90	3243.0
92.90	5016.0
93.90	14164.0
94.90	105552.0
95.90	7081.0
96.90	237.0
103.80	590.0
104.90	171.0
105.70	505.0
106.80	116.0
110.90	120.0
112.70	133.0
114.70	115.0
115.90	447.0
116.80	715.0
117.70	412.0
118.80	544.0
127.90	384.0
128.80	231.0
129.80	393.0
130.70	111.0
134.70	177.0
136.70	225.0
140.80	1221.0
141.80	124.0
142.80	1277.0
144.70	148.0
145.70	152.0
147.70	228.0
154.80	261.0
156.80	200.0
158.60	106.0
160.70	107.0
171.80	517.0
172.90	686.0
173.80	82960.0
174.80	6268.0
175.80	79880.0
176.80	4871.0
177.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	721.0
36.90	4268.0
37.90	3712.0
38.90	1579.0
39.90	117.0
43.90	859.0
44.80	671.0
46.90	731.0
47.90	579.0
48.90	4116.0
49.90	18248.0
51.00	5780.0
52.00	285.0
54.90	333.0
55.90	1689.0
56.90	3030.0
59.90	905.0
60.90	4867.0
61.90	4645.0
63.00	3885.0
63.90	406.0
64.90	204.0
66.90	260.0
67.90	10204.0
69.00	10541.0
69.90	888.0
71.90	567.0
72.90	4937.0
73.90	17680.0
74.90	51456.0
75.90	4573.0
76.80	541.0
77.70	305.0
78.80	3804.0
79.80	1076.0
80.80	3857.0
81.90	830.0
82.90	124.0
86.90	4047.0
87.90	3836.0
90.70	381.0
91.90	2945.0
92.90	4490.0
93.90	13281.0
94.90	99448.0
95.90	6322.0
96.90	237.0
103.80	487.0
104.90	179.0
105.70	448.0
106.80	109.0
110.80	113.0
112.70	120.0
114.70	145.0
115.90	418.0
116.80	641.0
117.80	413.0
118.80	539.0
127.90	367.0
128.80	221.0
129.80	380.0
134.70	186.0
136.70	221.0
140.80	1169.0
141.80	116.0
142.80	1261.0
144.70	126.0
145.80	144.0
147.70	229.0
154.80	286.0
156.80	167.0
171.80	496.0
172.80	683.0
173.80	80400.0
174.80	5807.0
175.80	77480.0
176.80	4506.0
177.80	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018