

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051753.D
 Acq On : 04 Nov 2022 12:16
 Operator : JC/MD
 Sample : N5407-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Z4

Quant Time: Nov 04 22:05:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	170574	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	184840	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	87365	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	55217	4.298	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.000%
7) Chloroethane-d5	1.912	69	53793	4.015	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.200%
11) 1,1-Dichloroethene-d2	2.562	65	22234	4.769	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.400%
20) 2-Butanone-d5	4.616	46	181055	38.915	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.840%
24) Chloroform-d	5.060	84	131559	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.700	65	67550	4.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
32) Benzene-d6	5.726	84	239253	4.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.690	67	84822	4.159	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.200%
41) Toluene-d8	7.896	98	184347	4.019	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%
43) trans-1,3-Dichloroprop...	8.179	79	26751	4.289	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.800%
46) 2-Hexanone-d5	8.632	63	137829	36.712	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.420%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	78262	4.187	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	78735	4.910	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.200%
Target Compounds					Qvalue	
13) Acetone	2.626	43	9022	3.822	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051753.D
Acq On : 04 Nov 2022 12:16
Operator : JC/MD
Sample : N5407-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Z4

Quant Time: Nov 04 22:05:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

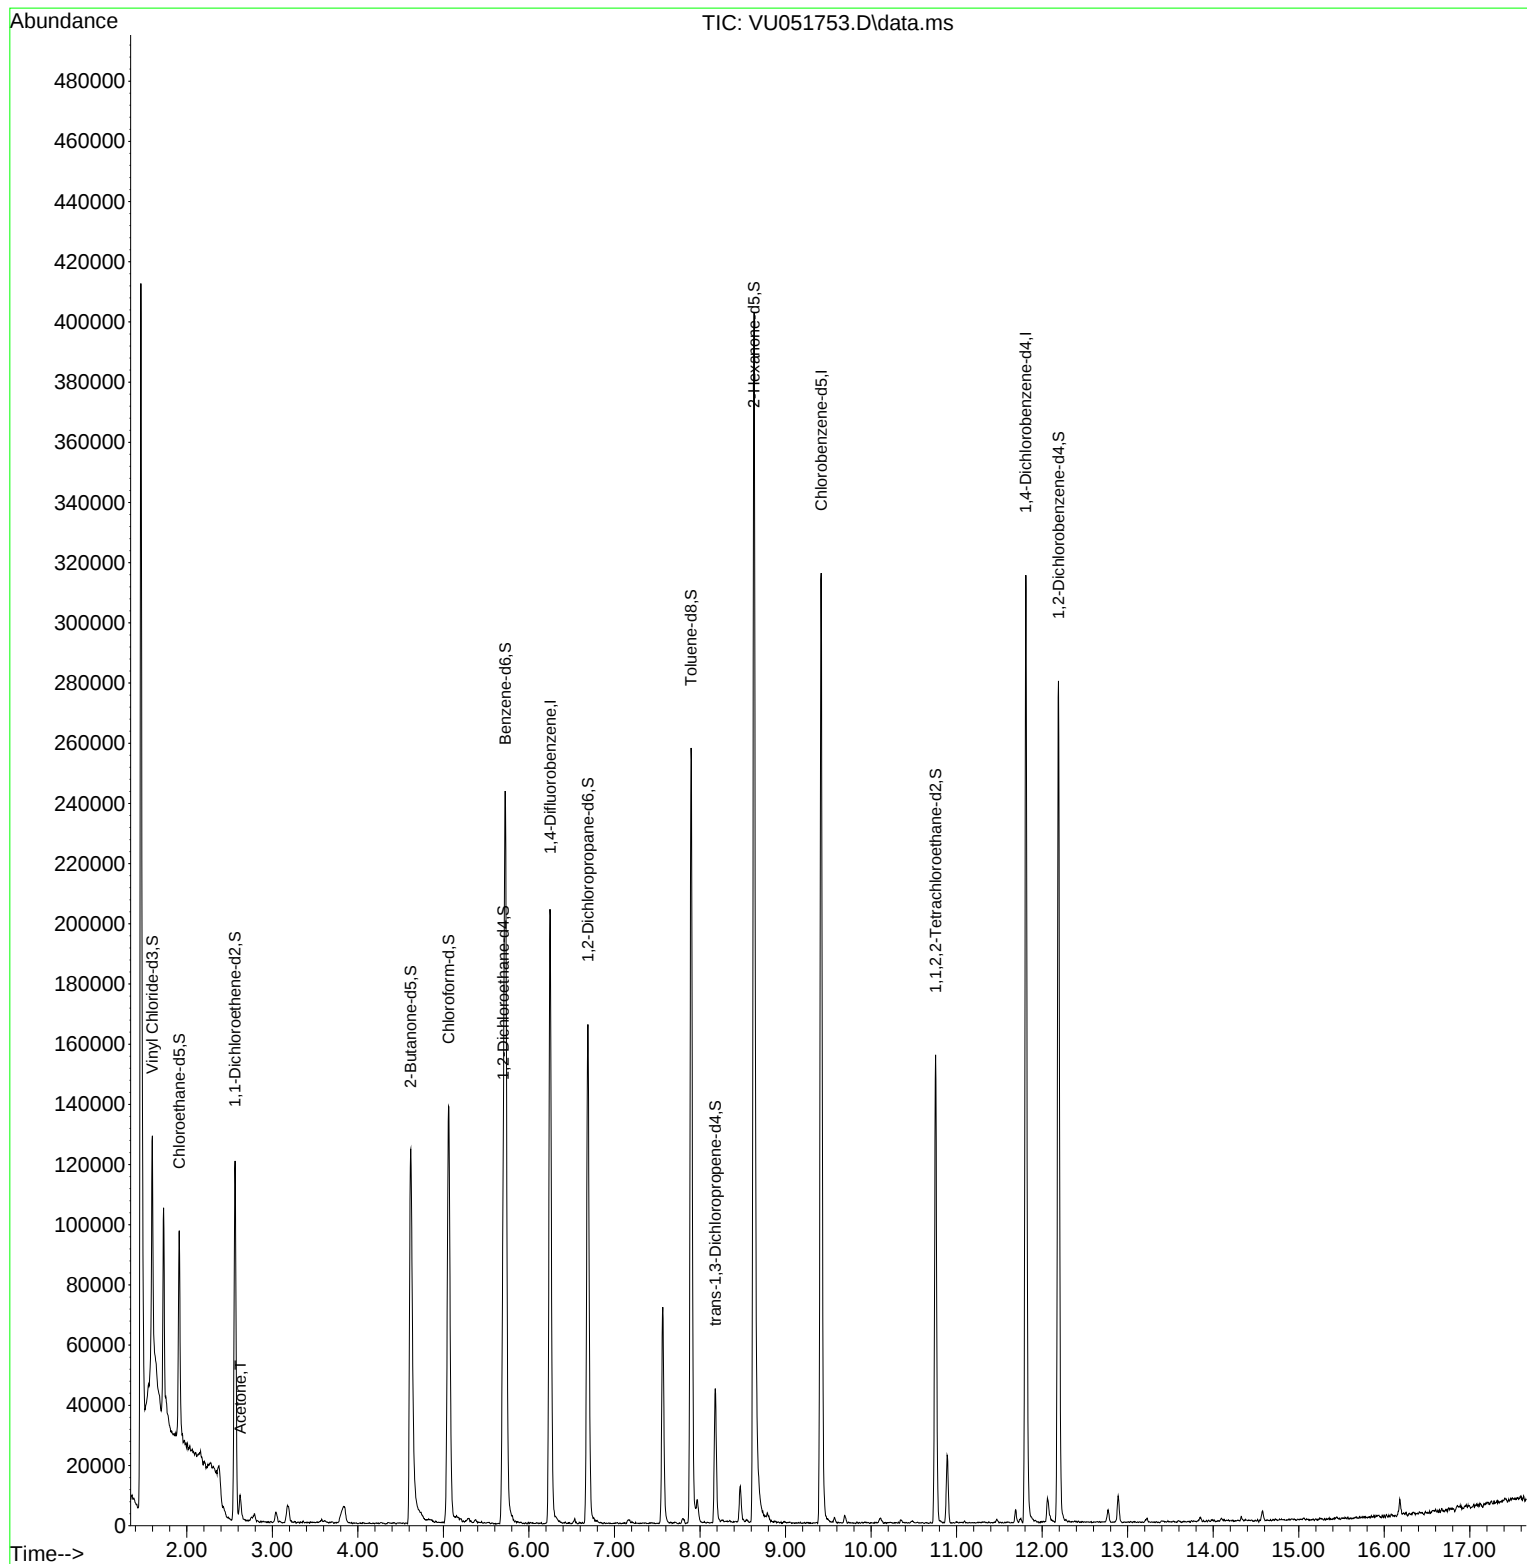

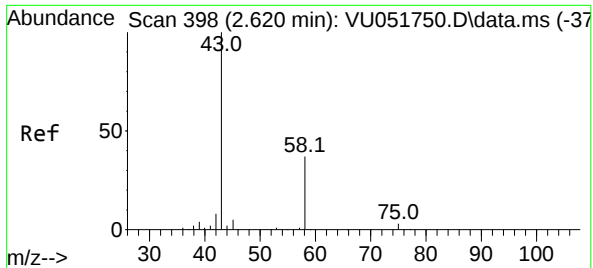

#13
 Acetone
 Concen: 3.822 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU051753.D
 Acq: 04 Nov 2022 12:16

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Z4

Tgt Ion: 43 Resp: 9022
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 73.8

