

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051754.D
 Acq On : 04 Nov 2022 12:41
 Operator : JC/MD
 Sample : N5407-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Z3

Quant Time: Nov 04 22:05:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	182655	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	199343	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	93370	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	53799	3.911	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.913	69	54938	3.829	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	2.565	65	22405	4.488	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.800%
20) 2-Butanone-d5	4.617	46	185365	37.206	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.420%
24) Chloroform-d	5.064	84	130314	4.048	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.000%
26) 1,2-Dichloroethane-d4	5.700	65	68710	3.951	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
32) Benzene-d6	5.726	84	236761	3.764	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.200%
36) 1,2-Dichloropropane-d6	6.690	67	82904	3.769	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	75.400%
41) Toluene-d8	7.896	98	185205	3.744	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	8.176	79	26510	3.941	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.800%
46) 2-Hexanone-d5	8.633	63	141646	34.984	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	69.960%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	79899	3.964	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	76855	4.485	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%
Target Compounds					Qvalue	
13) Acetone	2.626	43	6331	2.505	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051754.D
Acq On : 04 Nov 2022 12:41
Operator : JC/MD
Sample : N5407-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Z3

Quant Time: Nov 04 22:05:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

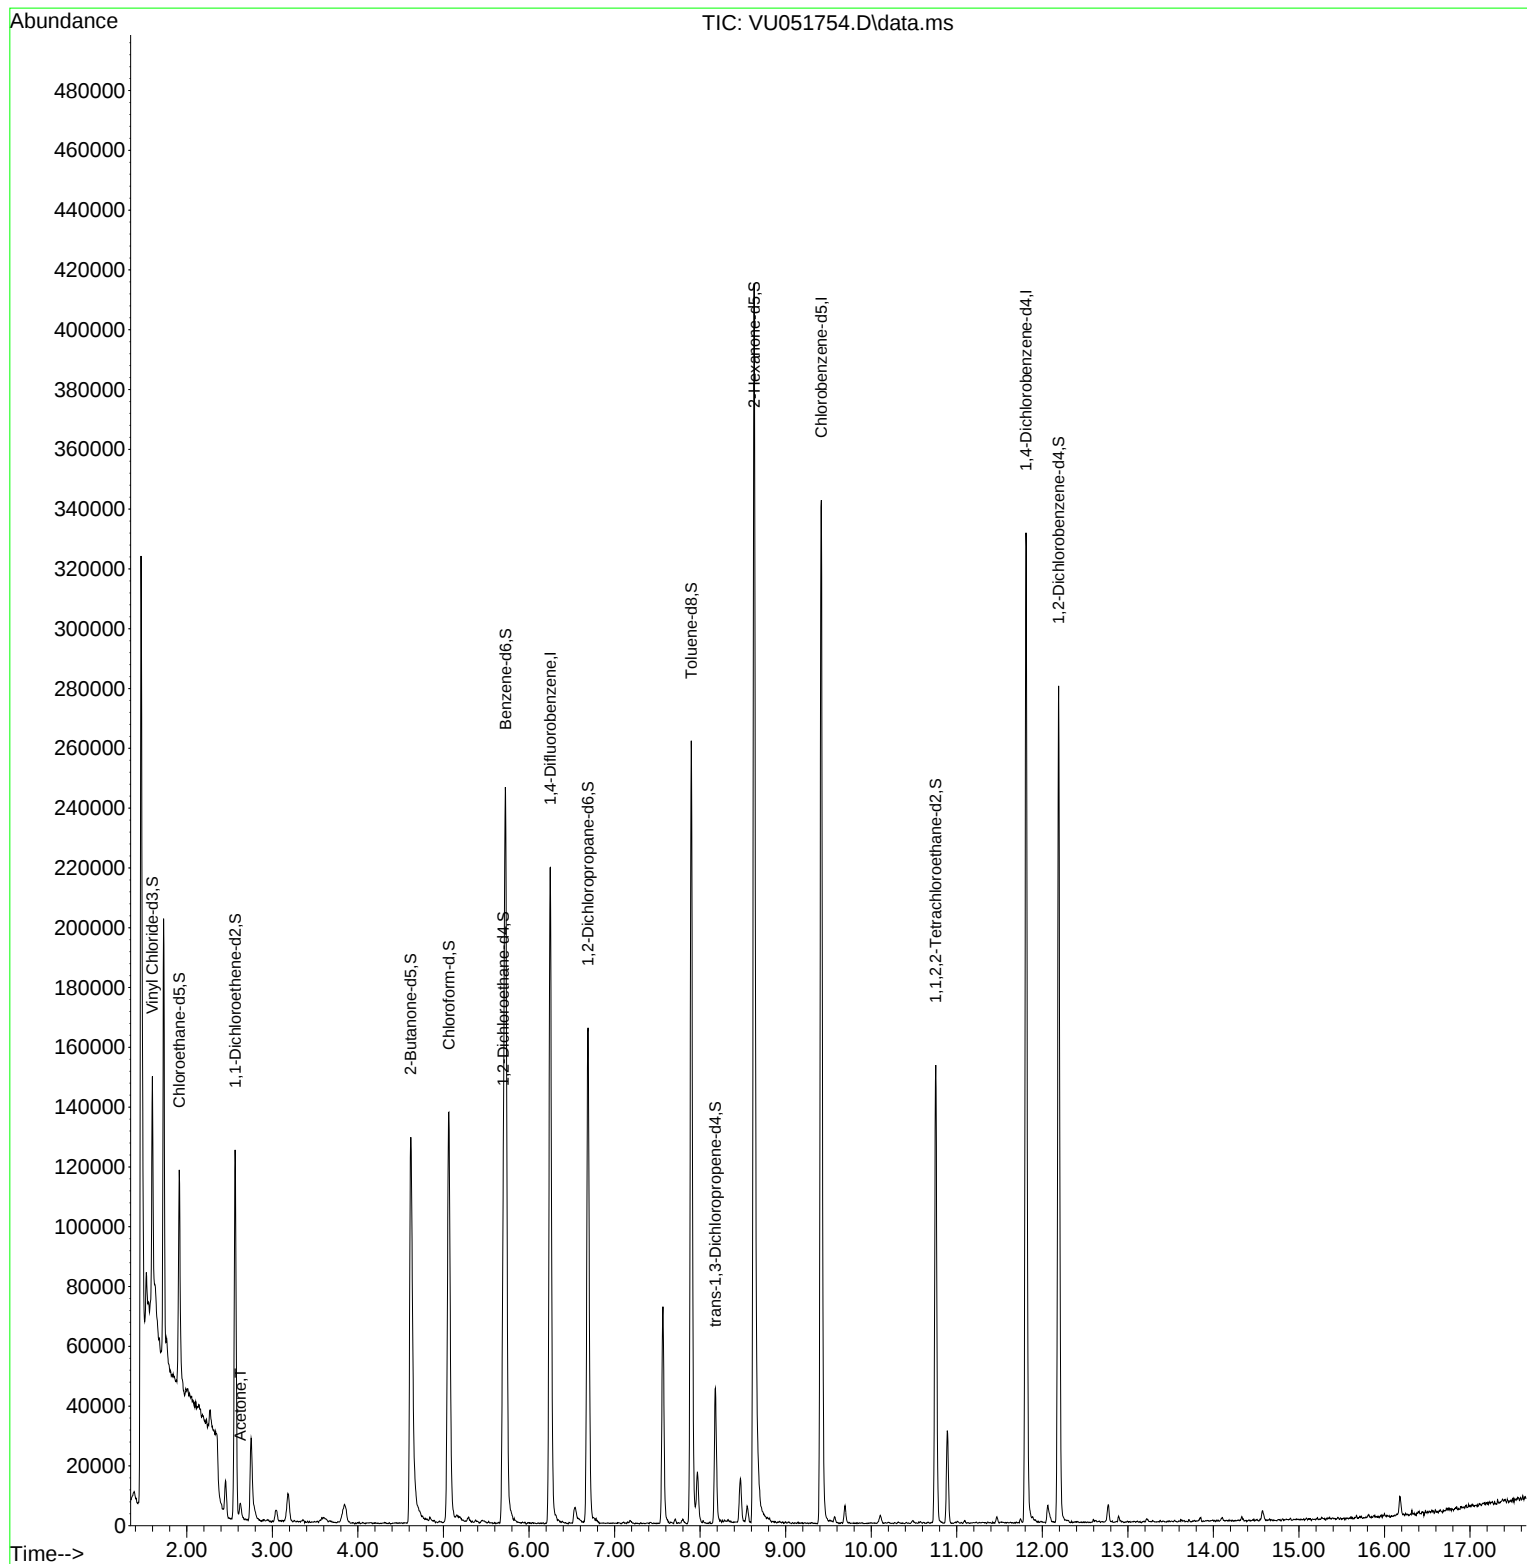

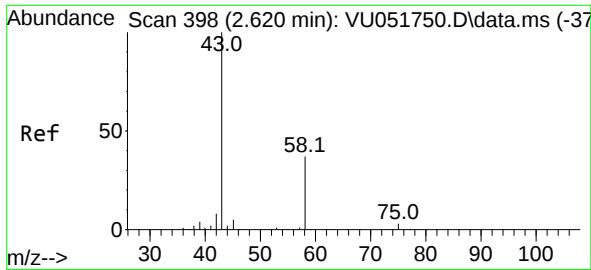

#13

Acetone

Concen: 2.505 ug/L

RT: 2.626 min Scan# 40

Delta R.T. 0.007 min

Lab File: VU051754.D

Acq: 04 Nov 2022 12:41

Instrument :

MSVOA_U

ClientSampleId :

EW4Z3

Tgt Ion: 43 Resp: 6331

Ion Ratio Lower Upper

43 100

58 39.0 0.0 73.8

