

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051758.D
 Acq On : 04 Nov 2022 14:19
 Operator : JC/MD
 Sample : N5407-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Y9

Quant Time: Nov 04 22:06:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	169093	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	188056	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	86408	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50369	3.955	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.912	69	50807	3.825	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	2.565	65	21736	4.703	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.000%
20) 2-Butanone-d5	4.620	46	173536	37.626	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.260%
24) Chloroform-d	5.060	84	127594	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
26) 1,2-Dichloroethane-d4	5.700	65	65942	4.096	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
32) Benzene-d6	5.726	84	223513	3.766	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.400%
36) 1,2-Dichloropropane-d6	6.690	67	82851	3.993	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.800%
41) Toluene-d8	7.896	98	170762	3.659	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%
43) trans-1,3-Dichloroprop...	8.176	79	24453	3.854	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.000%
46) 2-Hexanone-d5	8.629	63	130105	34.062	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.120%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	75662	3.979	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	73570	4.639	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds					Qvalue	
13) Acetone	2.626	43	10492	4.483	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051758.D
Acq On : 04 Nov 2022 14:19
Operator : JC/MD
Sample : N5407-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Y9

Quant Time: Nov 04 22:06:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

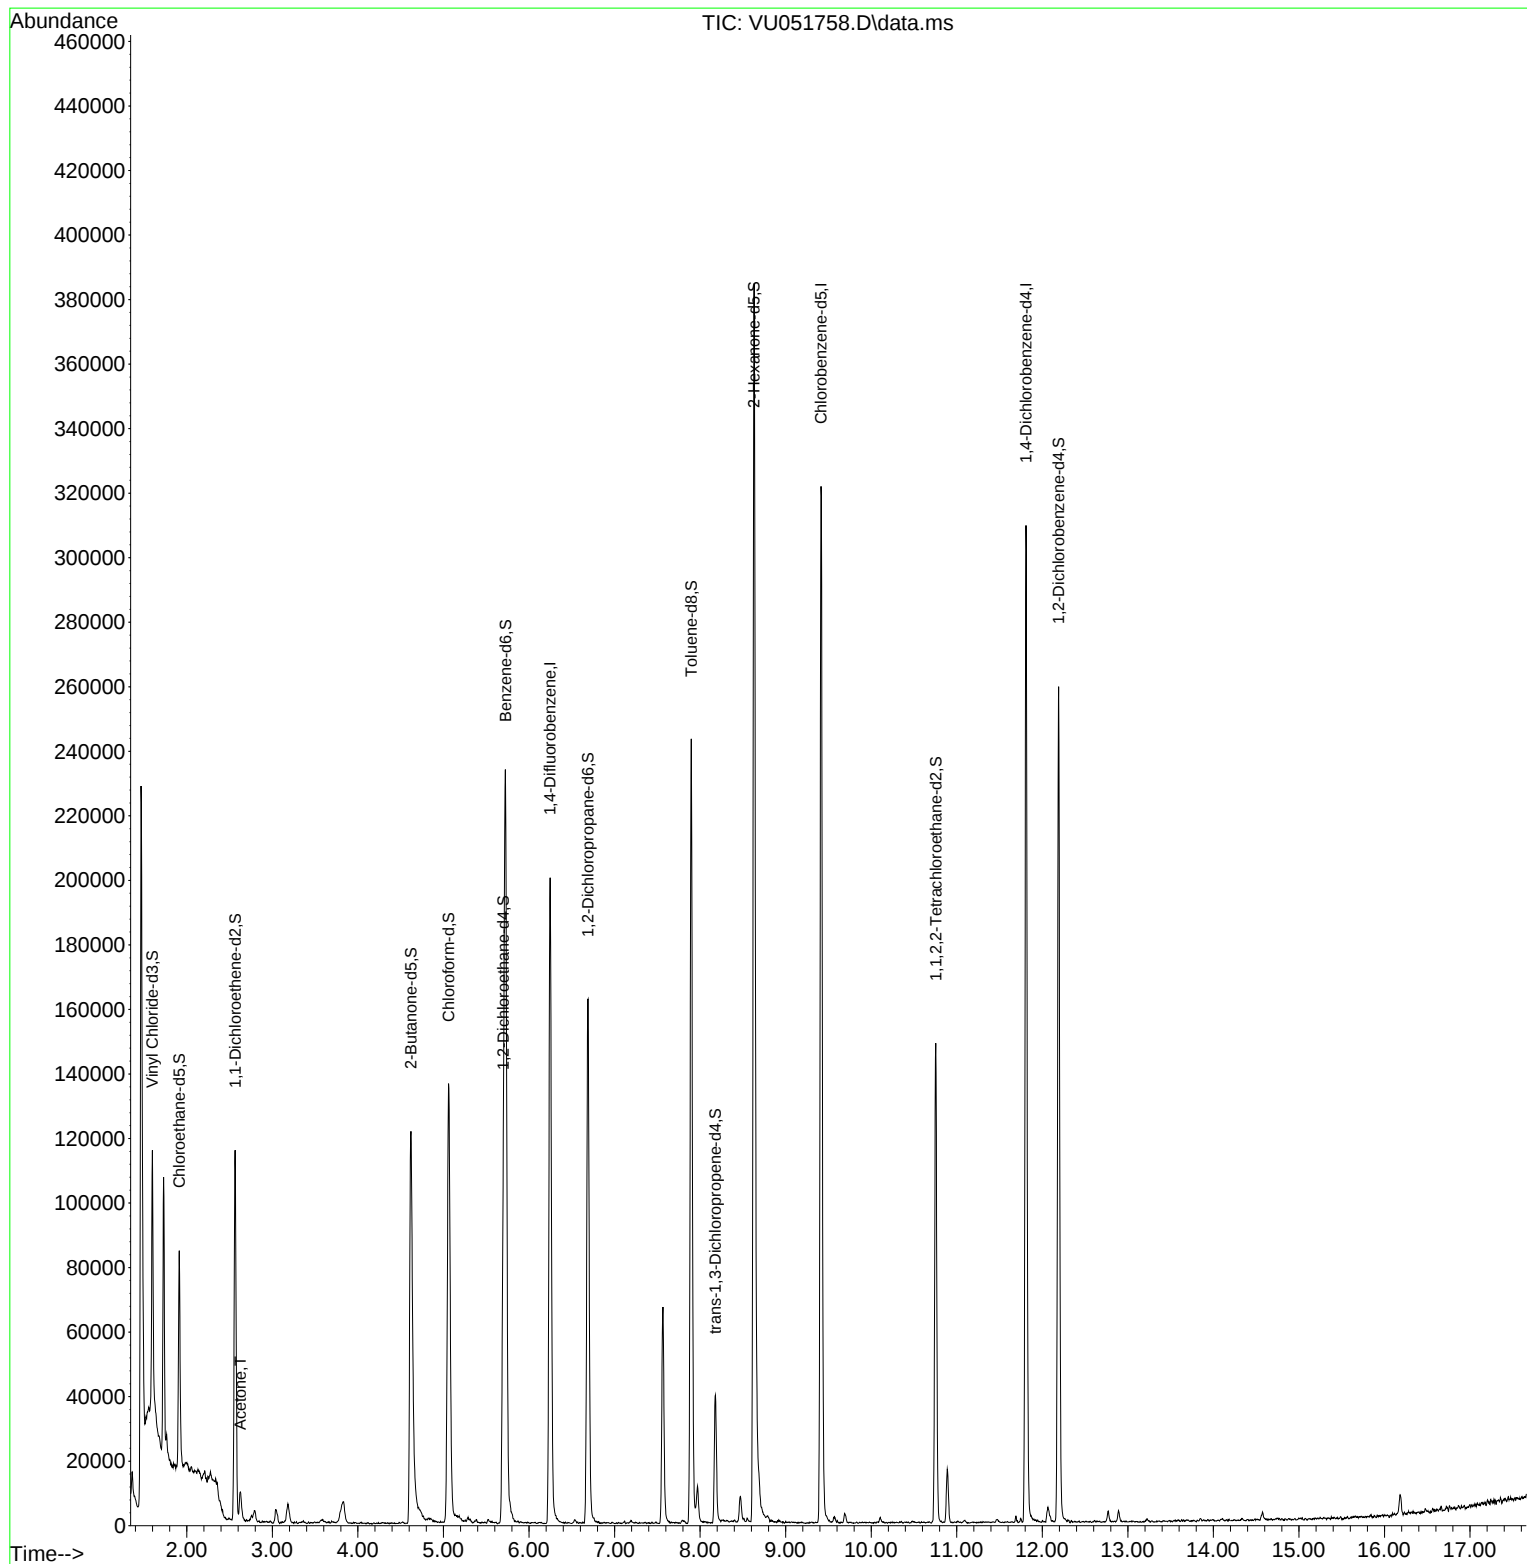

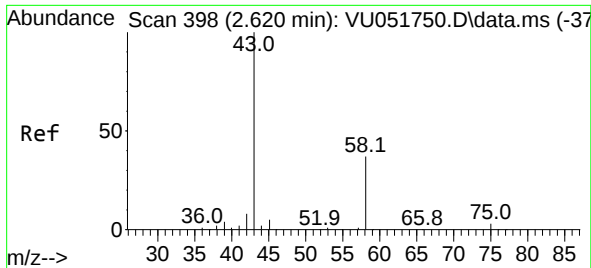

#13
 Acetone
 Concen: 4.483 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU051758.D
 Acq: 04 Nov 2022 14:19

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Y9

Tgt Ion: 43 Resp: 10492
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 73.8

