

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051759.D
 Acq On : 04 Nov 2022 14:45
 Operator : JC/MD
 Sample : N5407-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Z0

Quant Time: Nov 04 22:06:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	165298	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	184173	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	86468	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	49832	4.003	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.913	69	49643	3.823	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	2.565	65	20771	4.597	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.000%
20) 2-Butanone-d5	4.620	46	170590	37.836	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.680%
24) Chloroform-d	5.060	84	123170	4.228	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.700	65	64019	4.068	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
32) Benzene-d6	5.726	84	223091	3.838	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.800%
36) 1,2-Dichloropropane-d6	6.690	67	81782	4.024	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.400%
41) Toluene-d8	7.896	98	166251	3.637	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.800%
43) trans-1,3-Dichloroprop...	8.179	79	24408	3.928	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.600%
46) 2-Hexanone-d5	8.632	63	127372	34.050	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.100%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	73344	3.938	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	72310	4.556	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds					Qvalue	
13) Acetone	2.626	43	8228	3.597	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051759.D
Acq On : 04 Nov 2022 14:45
Operator : JC/MD
Sample : N5407-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Z0

Quant Time: Nov 04 22:06:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

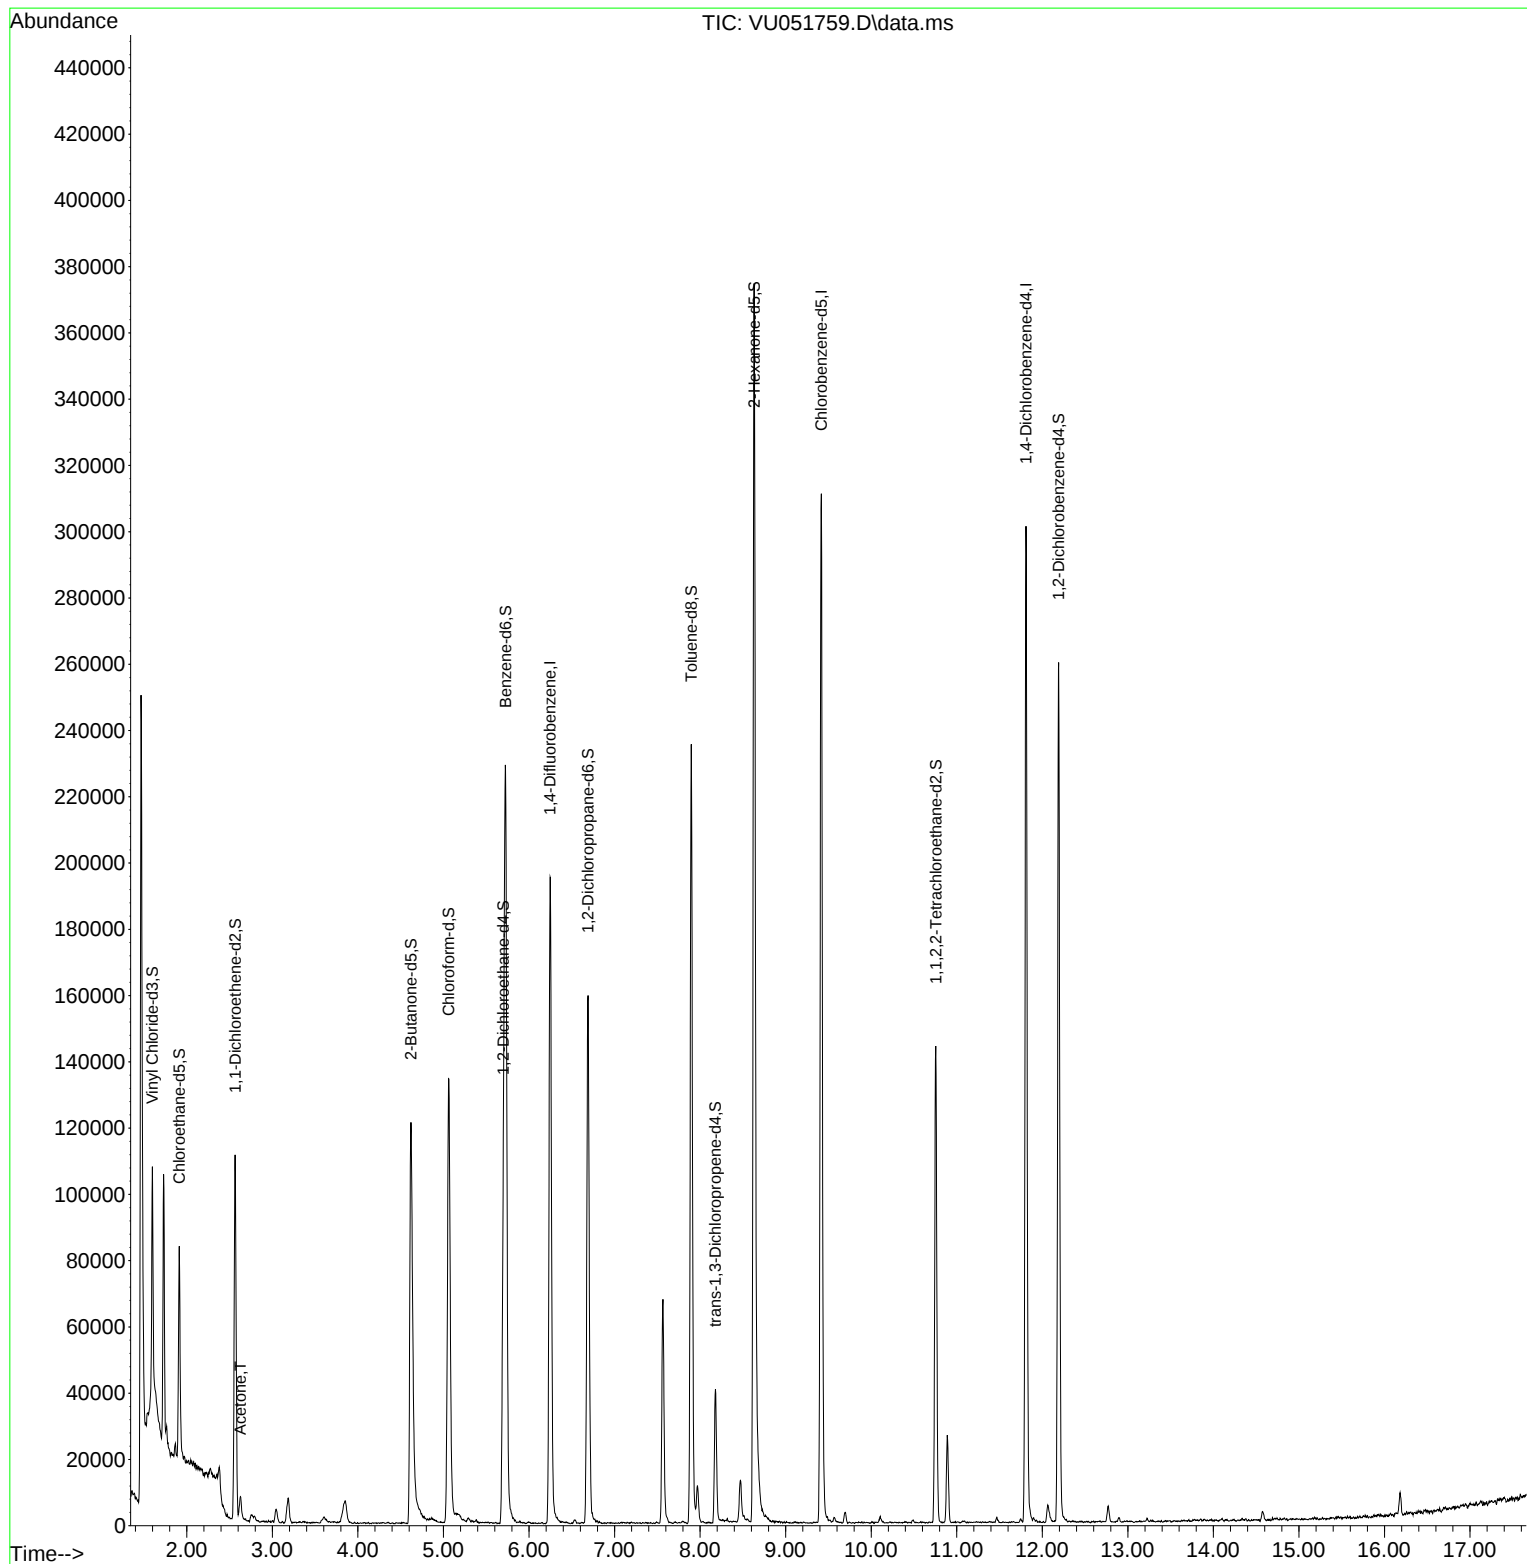

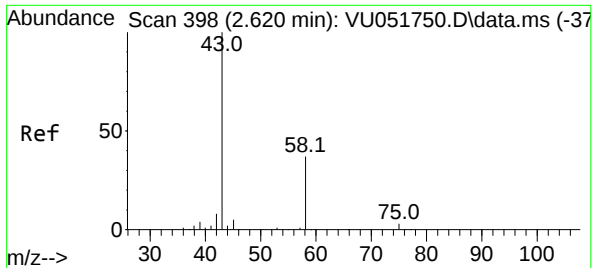

#13
 Acetone
 Concen: 3.597 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.007 min
 Lab File: VU051759.D
 Acq: 04 Nov 2022 14:45

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Z0

Tgt Ion: 43 Resp: 8228
 Ion Ratio Lower Upper
 43 100
 58 34.8 0.0 73.8

