

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051762.D
 Acq On : 04 Nov 2022 16:00
 Operator : JC/MD
 Sample : N5407-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Y3

Quant Time: Nov 04 22:07:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	142544	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	158016	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	72089	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43556	4.057	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.912	69	45426	4.057	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.200%
11) 1,1-Dichloroethene-d2	2.565	65	18911	4.854	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.000%
20) 2-Butanone-d5	4.620	46	166881	42.922	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.840%
24) Chloroform-d	5.063	84	109498	4.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	5.700	65	58392	4.303	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	5.726	84	194978	3.910	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%
36) 1,2-Dichloropropane-d6	6.690	67	69234	3.971	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.400%
41) Toluene-d8	7.896	98	140680	3.588	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.800%
43) trans-1,3-Dichloroprop...	8.179	79	22663	4.251	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.632	63	119996	37.388	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.780%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	73450	4.597	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	62154	4.697	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.000%
Target Compounds					Qvalue	
13) Acetone	2.626	43	9700	4.917	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051762.D
Acq On : 04 Nov 2022 16:00
Operator : JC/MD
Sample : N5407-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Y3

Quant Time: Nov 04 22:07:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

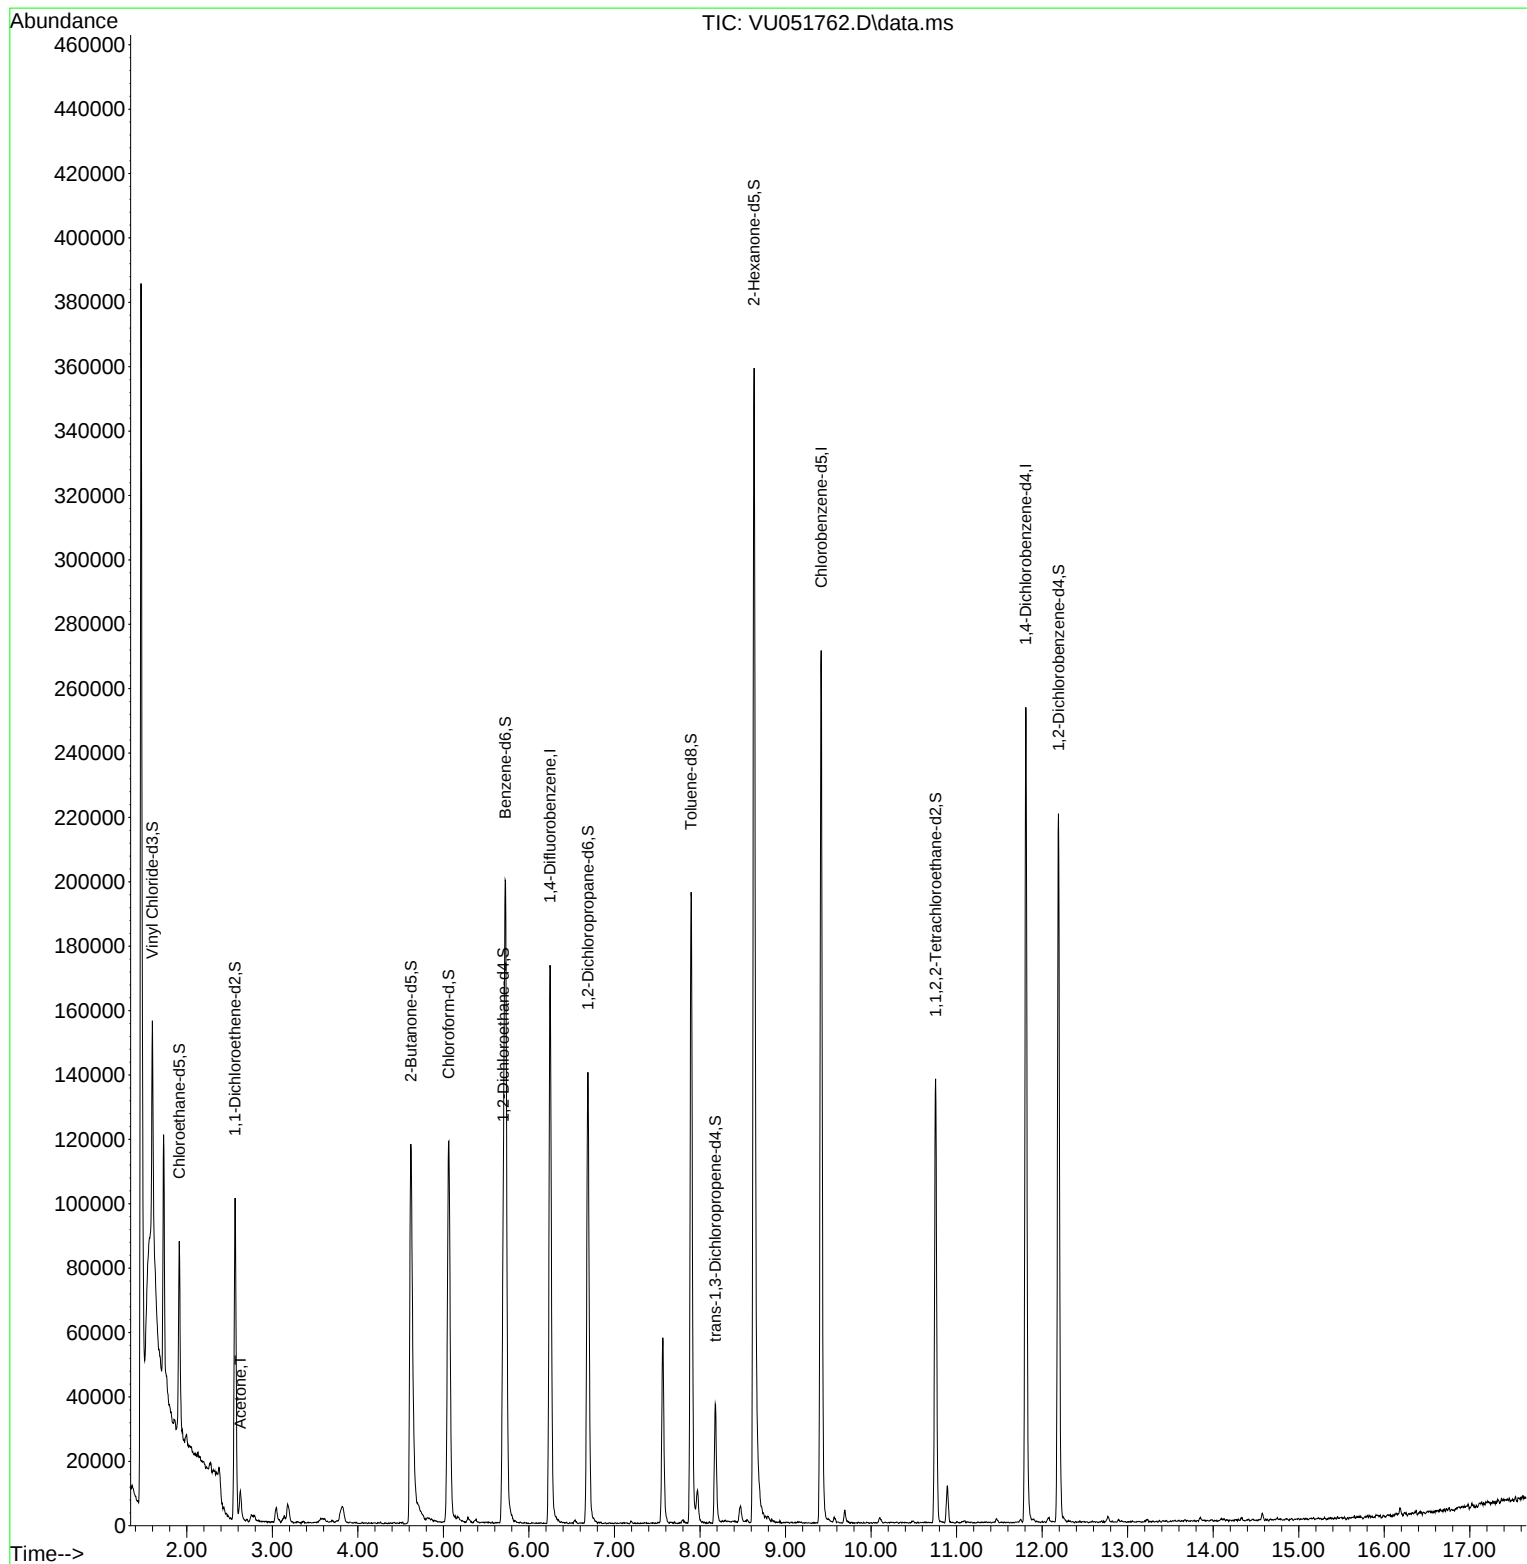

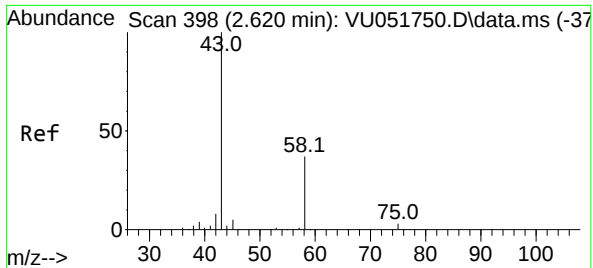

#13

Acetone

Concen: 4.917 ug/L

RT: 2.626 min Scan# 40

Delta R.T. 0.007 min

Lab File: VU051762.D

Acq: 04 Nov 2022 16:00

Instrument :

MSVOA_U

ClientSampleId :

EW4Y3

Tgt Ion: 43 Resp: 9700

Ion Ratio Lower Upper

43 100

58 37.5 0.0 73.8

