

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051764.D
 Acq On : 04 Nov 2022 16:49
 Operator : JC/MD
 Sample : N5407-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Nov 04 22:08:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 04 22:04:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	164089	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	183369	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	84647	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	48303	3.909	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.912	69	49263	3.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	2.562	65	20406	4.550	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.000%
20) 2-Butanone-d5	4.616	46	170477	38.090	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.180%
24) Chloroform-d	5.060	84	126887	4.388	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.700	65	63642	4.074	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
32) Benzene-d6	5.726	84	218506	3.776	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.600%
36) 1,2-Dichloropropane-d6	6.687	67	79707	3.939	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.800%
41) Toluene-d8	7.896	98	162789	3.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	8.179	79	23072	3.729	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%
46) 2-Hexanone-d5	8.632	63	126950	34.086	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	68.180%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	75681	4.082	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	71451	4.599	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%
Target Compounds						Qvalue
16) Methylene chloride	3.044	84	28159	1.205	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
Data File : VU051764.D
Acq On : 04 Nov 2022 16:49
Operator : JC/MD
Sample : N5407-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Nov 04 22:08:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 04 22:04:33 2022
Response via : Initial Calibration

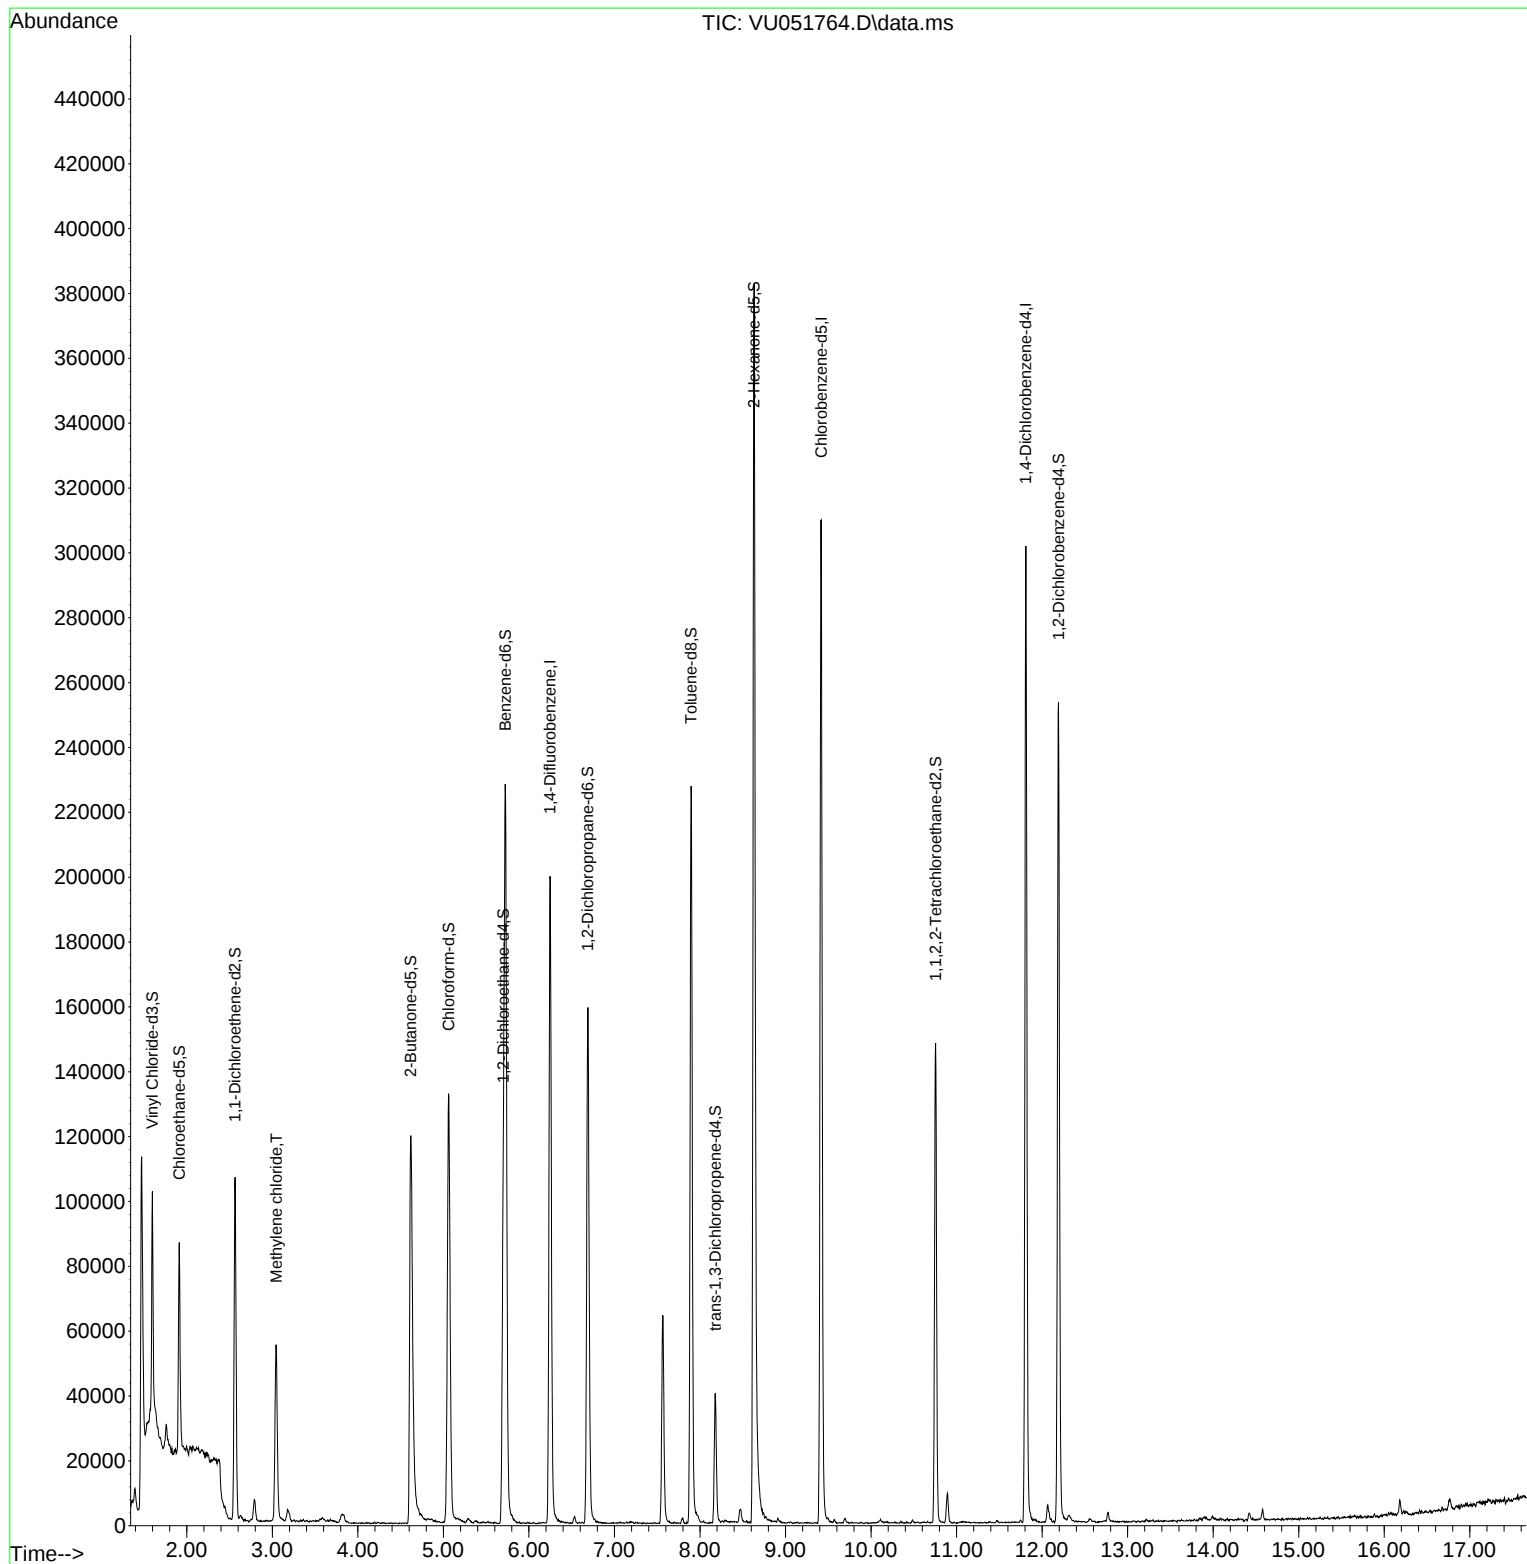

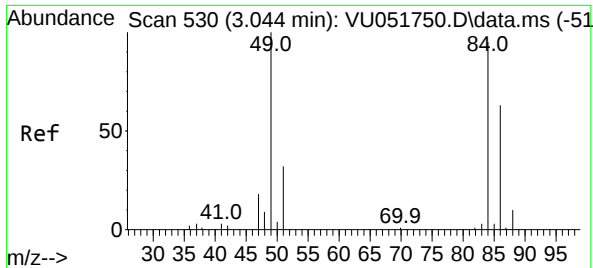

#16
Methylene chloride
Concen: 1.205 ug/L
RT: 3.044 min Scan# 51
Delta R.T. 0.000 min
Lab File: VU051764.D
Acq: 04 Nov 2022 16:49

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	28159
Ion	Ratio	Lower	Upper
84	100		
86	64.5	46.3	85.9
49	110.9	76.0	141.2

