


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110422\
 Data File : VU051749.D
 Acq On : 04 Nov 2022 09:00
 Operator : JC/MD
 Sample : BFB164
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB164

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 04 22:04:33 2022

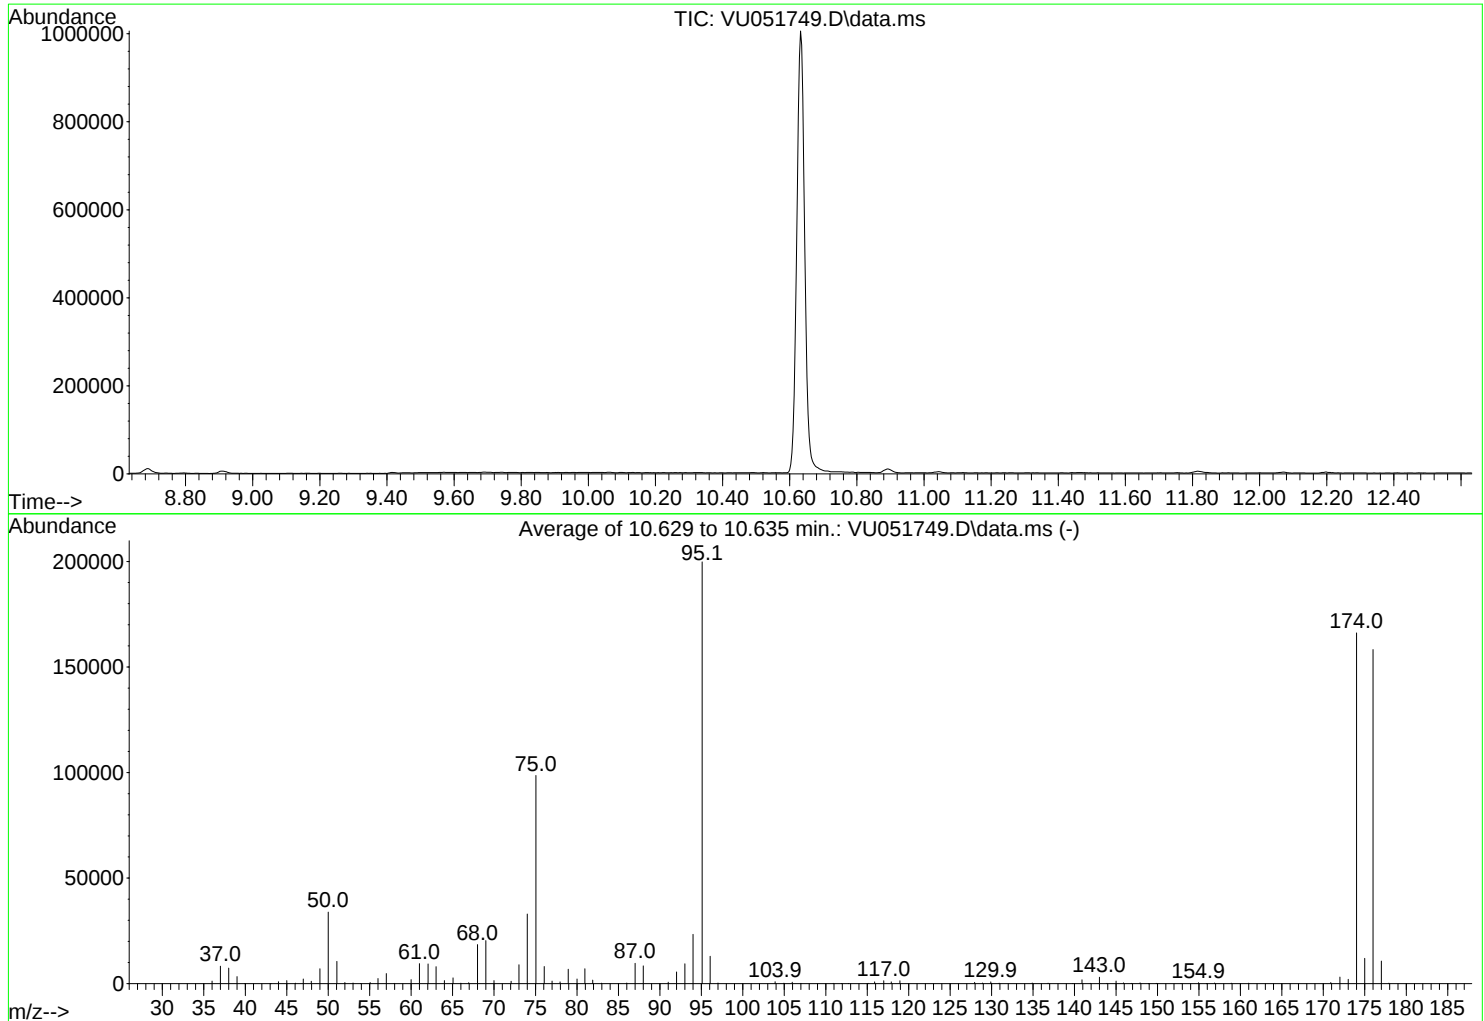

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	33875	PASS
75	95	30	80	49.4	98653	PASS
95	95	100	100	100.0	199829	PASS
96	95	5	9	6.5	13006	PASS
173	174	0.00	2	1.3	2082	PASS
174	95	50	120	83.2	166187	PASS
175	174	5	9	7.2	12012	PASS
176	174	95	101	95.2	158272	PASS
177	176	5	9	6.8	10704	PASS

m/z	Abundance
36.00	1103.0
37.00	103.0
38.00	384.0
39.90	652.0
44.00	466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.00	2364.0
37.00	8437.0
38.00	7896.0
39.00	3442.0
40.00	759.0
44.00	1358.0
45.00	1340.0
46.00	298.0
47.00	2176.0
48.00	1190.0
49.00	7019.0
50.00	33832.0
51.00	10659.0
52.00	523.0
53.00	319.0
55.00	549.0
56.00	2308.0
57.00	4954.0
57.90	165.0
60.00	1849.0
61.00	9749.0
62.10	9090.0
63.00	7865.0
64.00	1532.0
65.00	2591.0
66.00	155.0
67.00	521.0
68.00	18336.0
69.00	20304.0
70.00	1549.0
72.10	1141.0
73.00	8754.0
74.00	31952.0
75.10	96512.0
76.10	8089.0
77.00	1155.0
78.00	830.0
78.90	7080.0
80.00	2095.0
80.90	6747.0
81.90	1734.0
83.00	209.0
86.00	268.0
87.00	9690.0
88.00	8088.0
91.00	656.0
92.00	5244.0
93.00	9473.0
94.00	22472.0
95.10	194304.0
96.00	13049.0
97.00	341.0
103.90	874.0
105.00	247.0
105.90	748.0
107.00	142.0
110.90	182.0
112.80	121.0
115.10	145.0
115.90	798.0
117.00	1340.0
117.90	719.0
119.00	1349.0
127.90	638.0
128.90	319.0
129.90	901.0
130.90	206.0
134.90	249.0
136.80	171.0
140.90	1657.0
141.90	138.0
143.00	3060.0
143.90	154.0
145.00	1239.0
145.90	365.0
146.80	100.0
147.90	279.0
148.90	104.0
149.80	181.0
152.80	109.0
154.90	413.0
156.90	295.0
158.90	197.0
161.00	246.0
170.90	556.0
172.00	2953.0
173.00	1912.0
174.00	157632.0
175.00	11904.0
176.00	150272.0
177.00	10170.0
177.90	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.00	2415.0
37.00	8622.0
38.00	8094.0
39.00	3469.0
40.00	760.0
44.00	1398.0
45.00	1479.0
46.10	240.0
47.00	2269.0
48.00	1124.0
49.00	7270.0
50.00	34824.0
51.10	10823.0
52.00	530.0
53.00	341.0
53.90	128.0
55.00	507.0
56.00	2470.0
57.00	4902.0
57.90	166.0
60.00	1989.0
61.00	9697.0
62.10	9623.0
63.00	8317.0
64.00	1473.0
65.00	2855.0
66.00	270.0
67.00	500.0
68.00	19144.0
69.00	21048.0
70.00	1487.0
72.00	1123.0
73.00	9225.0
74.00	34032.0
75.00	101792.0
76.10	8488.0
77.00	1236.0
78.00	917.0
78.90	7097.0
80.00	2324.0
80.90	7187.0
81.90	1741.0
83.00	210.0
86.00	332.0
87.00	10038.0
88.00	8732.0
91.00	732.0
92.00	5785.0
93.00	9796.0
94.00	24184.0
95.10	205760.0
96.00	13492.0
97.00	325.0
103.90	966.0
104.90	271.0
105.90	757.0
107.00	196.0
110.90	179.0
111.90	109.0
112.80	115.0
115.10	158.0
115.90	860.0
117.00	1415.0
117.90	868.0
118.90	1389.0
127.90	626.0
128.90	305.0
129.90	910.0
130.90	216.0
134.90	337.0
136.80	223.0
139.80	117.0
140.90	1913.0
141.90	168.0
143.00	3116.0
143.90	157.0
145.00	1272.0
145.90	384.0
146.80	142.0
147.90	382.0
149.80	182.0
152.80	129.0
155.00	439.0
156.90	288.0
158.90	225.0
161.00	265.0
170.90	562.0
172.00	3272.0
173.00	2165.0
174.00	171072.0
175.00	12395.0
176.00	163520.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

177.0011025.0

177.90286.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

m/z	Abundance
36.00	2261.0
37.00	8025.0
38.00	7295.0
39.00	3197.0
40.00	709.0
43.00	135.0
44.00	1424.0
45.00	1510.0
46.10	204.0
47.00	2182.0
47.90	1122.0
49.00	6957.0
50.00	32968.0
51.10	10252.0
52.00	522.0
53.00	273.0
53.90	152.0
55.10	432.0
56.00	2417.0
57.00	4580.0
58.00	170.0
60.00	1917.0
61.00	8905.0
62.00	9164.0
63.00	7930.0
64.00	1293.0
65.10	2777.0
66.00	357.0
66.90	406.0
68.00	18048.0
69.00	19768.0
70.00	1396.0
72.00	1097.0
73.00	8770.0
74.00	32936.0
75.00	97656.0
76.00	7862.0
77.00	1257.0
77.90	882.0
79.00	6301.0
80.00	2275.0
81.00	7166.0
81.90	1640.0
82.90	159.0
86.00	326.0
87.00	9247.0
88.00	8537.0
91.00	704.0
92.00	5646.0
93.00	9007.0
94.00	23304.0
95.10	199424.0
96.10	12478.0
97.00	255.0
103.90	968.0
104.90	256.0
106.00	671.0
107.00	218.0
110.90	165.0
111.90	129.0
112.70	105.0
115.10	139.0
115.90	798.0
117.00	1376.0
117.90	840.0
118.90	1381.0
128.00	644.0
128.90	260.0
129.90	793.0
130.90	215.0
134.90	419.0
136.80	266.0
139.80	139.0
140.90	1998.0
141.90	217.0
143.00	2851.0
143.90	149.0
145.00	1254.0
145.90	352.0
146.90	148.0
147.90	486.0
149.90	175.0
152.90	119.0
155.00	435.0
155.90	121.0
156.90	256.0
158.90	205.0
161.00	248.0
170.90	532.0
172.00	3148.0
173.00	2169.0
174.00	169856.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164

175.00	11736.0
176.00	161024.0
177.00	10916.0
177.90	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB164