




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061431.D
Acq On : 05 Nov 2024 01:44
Operator : MD/SY
Sample : P4691-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CQ8

Manual IntegrationsAPPROVED

Quant Time: Nov 05 04:53:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 05 04:38:45 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
Supervised By :Mahesh Dadoda 11/06/2024

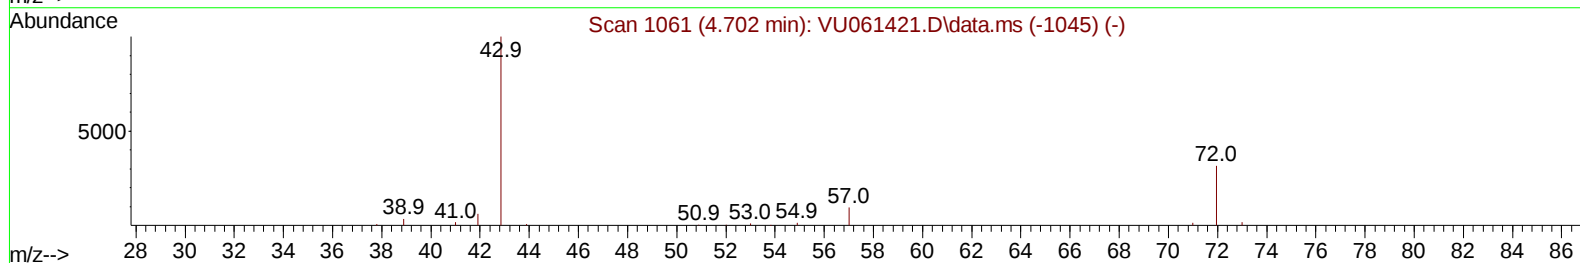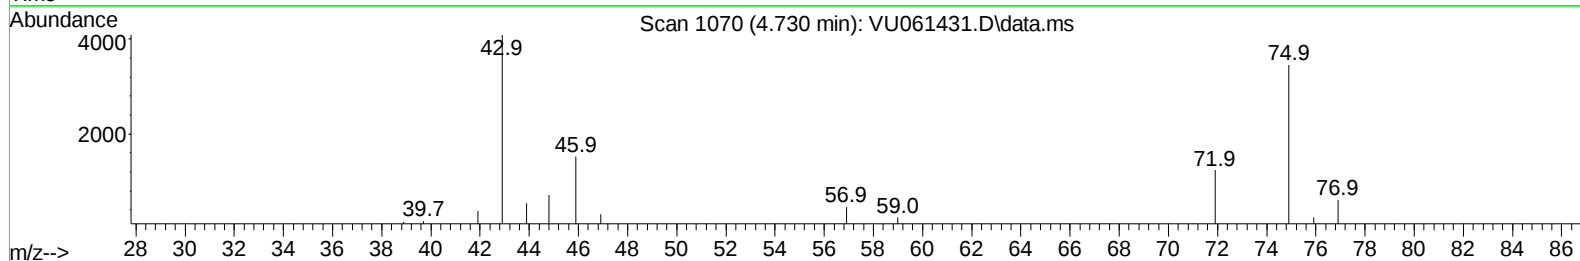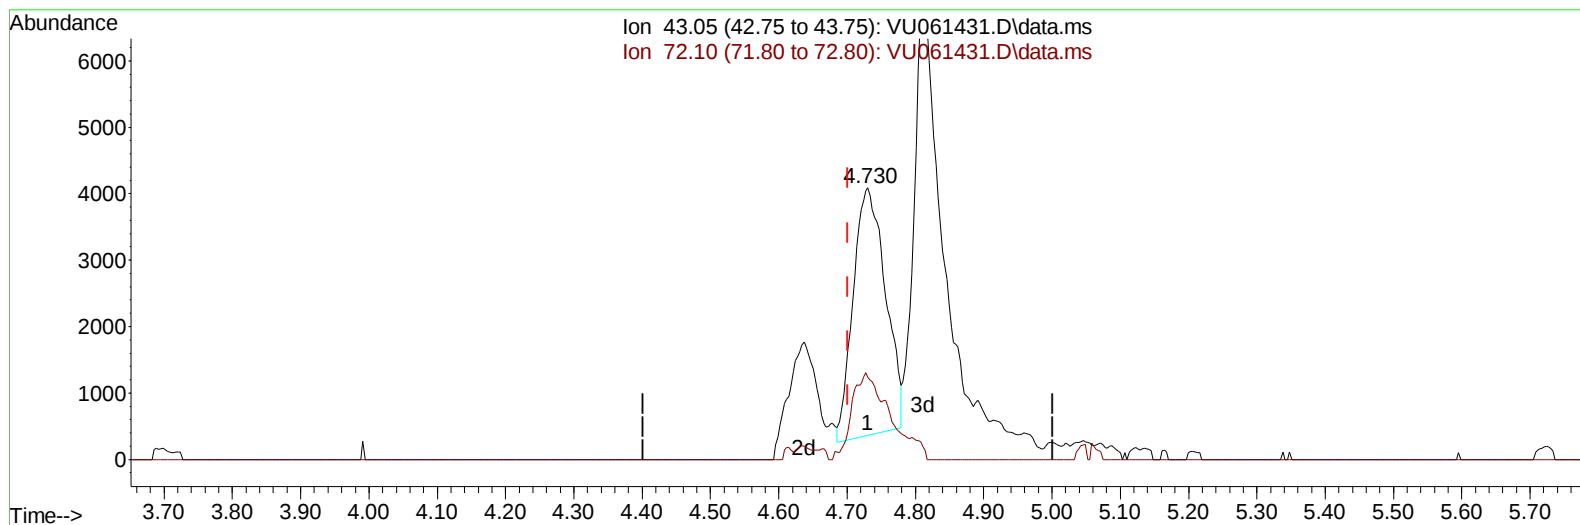

TIC: VU061431.D\data.ms

(21) 2-Butanone (T)

4.730min (+ 0.029) 5.68 ug/L

response 12194

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	31.70	41.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
 Data File : VU061431.D
 Acq On : 05 Nov 2024 01:44
 Operator : MD/SY
 Sample : P4691-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CQ8

Manual IntegrationsAPPROVED

Quant Time: Nov 05 04:53:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 05 04:38:45 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
 Supervised By :Mahesh Dadoda 11/06/2024

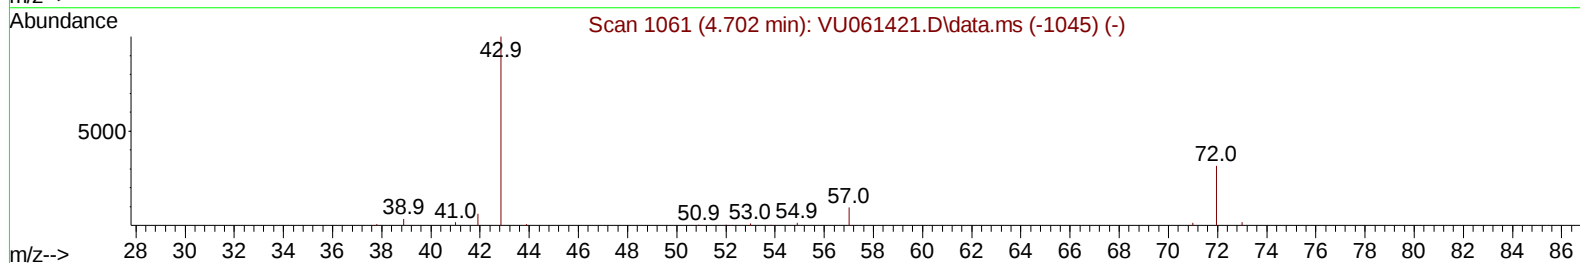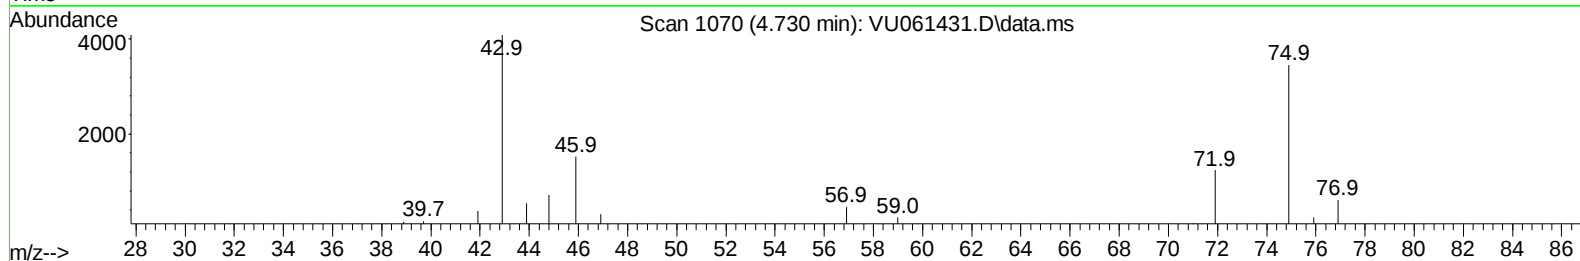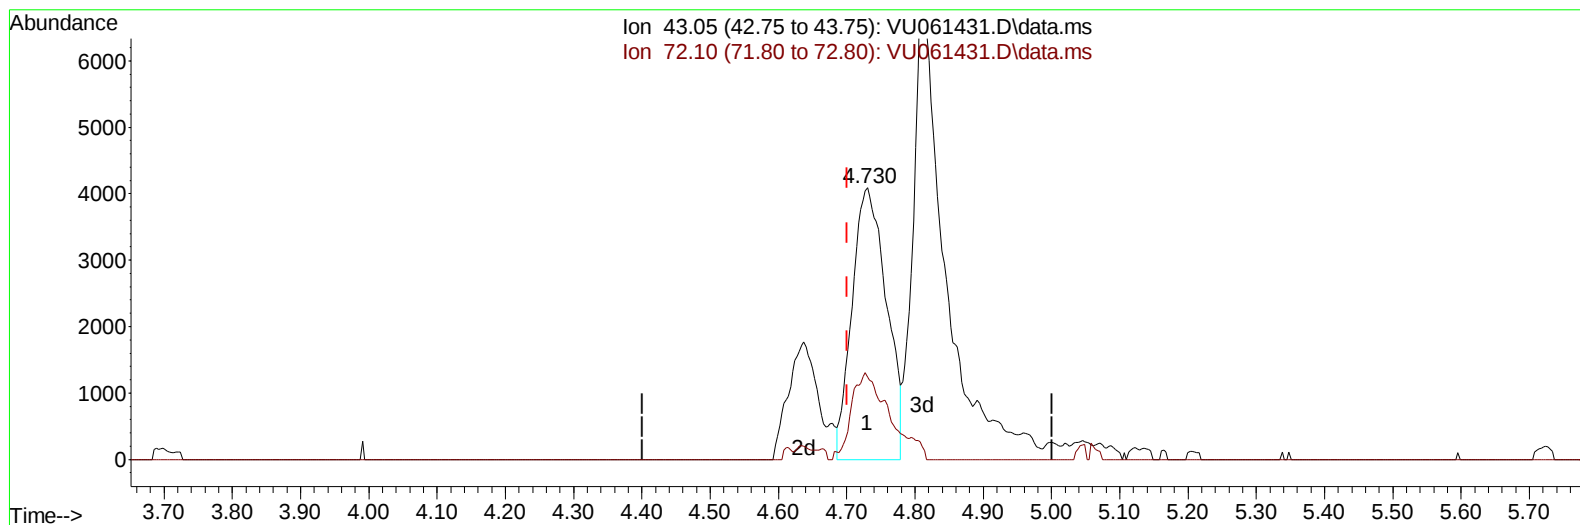

TIC: VU061431.D\data.ms

(21) 2-Butanone (T)

4.730min (+ 0.029) 6.64 ug/L m

response 14247

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	31.70	35.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
 Data File : VU061431.D
 Acq On : 05 Nov 2024 01:44
 Operator : MD/SY
 Sample : P4691-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CQ8

Manual IntegrationsAPPROVED

Quant Time: Nov 05 04:53:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 05 04:38:45 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
 Supervised By :Mahesh Dadoda 11/06/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		154936	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		145308	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152		63381	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		29609	2.813	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	56.200%	
7) Chloroethane-d5	1.911	69		29537	3.061	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	61.200%#	
11) 1,1-Dichloroethene-d2	2.560	65		14876	3.304	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	66.000%	
20) 2-Butanone-d5	4.631	46		99790	46.700	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	93.400%	
24) Chloroform-d	5.052	84		79999	4.004	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	80.000%	
26) 1,2-Dichloroethane-d4	5.695	65		41868	4.205	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	84.000%	
32) Benzene-d6	5.718	84		160550	3.921	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	78.400%	
36) 1,2-Dichloropropane-d6	6.682	67		49926	4.056	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	81.200%	
41) Toluene-d8	7.891	98		138508	3.618	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	72.400%	
43) trans-1,3-Dichloroprop...	8.174	79		15857	3.156	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	63.200%	
46) 2-Hexanone-d5	8.627	63		82296	39.988	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	79.980%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84		39514	4.245	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	84.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		48816	4.349	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	87.000%	
Target Compounds							
13) Acetone	2.660	43		9834	7.266	ug/L	98
21) 2-Butanone	4.730	43		14247m	6.640	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061431.D
Acq On : 05 Nov 2024 01:44
Operator : MD/SY
Sample : P4691-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CQ8

Manual IntegrationsAPPROVED

Quant Time: Nov 05 04:53:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 05 04:38:45 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
Supervised By :Mahesh Dadoda 11/06/2024

