




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061442.D
Acq On : 05 Nov 2024 06:14
Operator : MD/SY
Sample : P4689-11
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD3

Manual IntegrationsAPPROVED

Quant Time: Nov 05 06:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 05 04:38:45 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
Supervised By :Mahesh Dadoda 11/06/2024

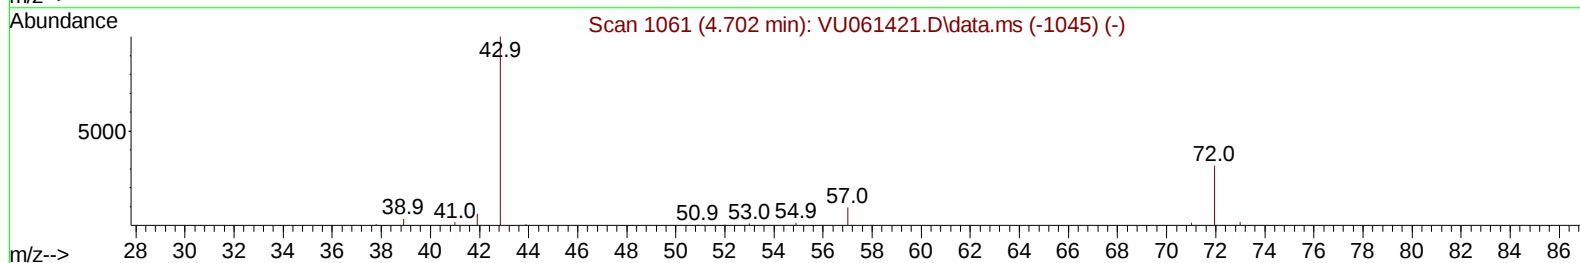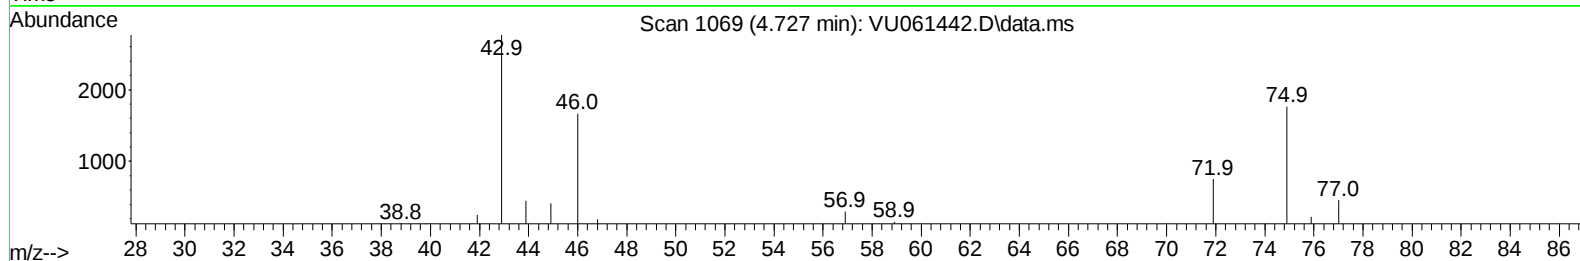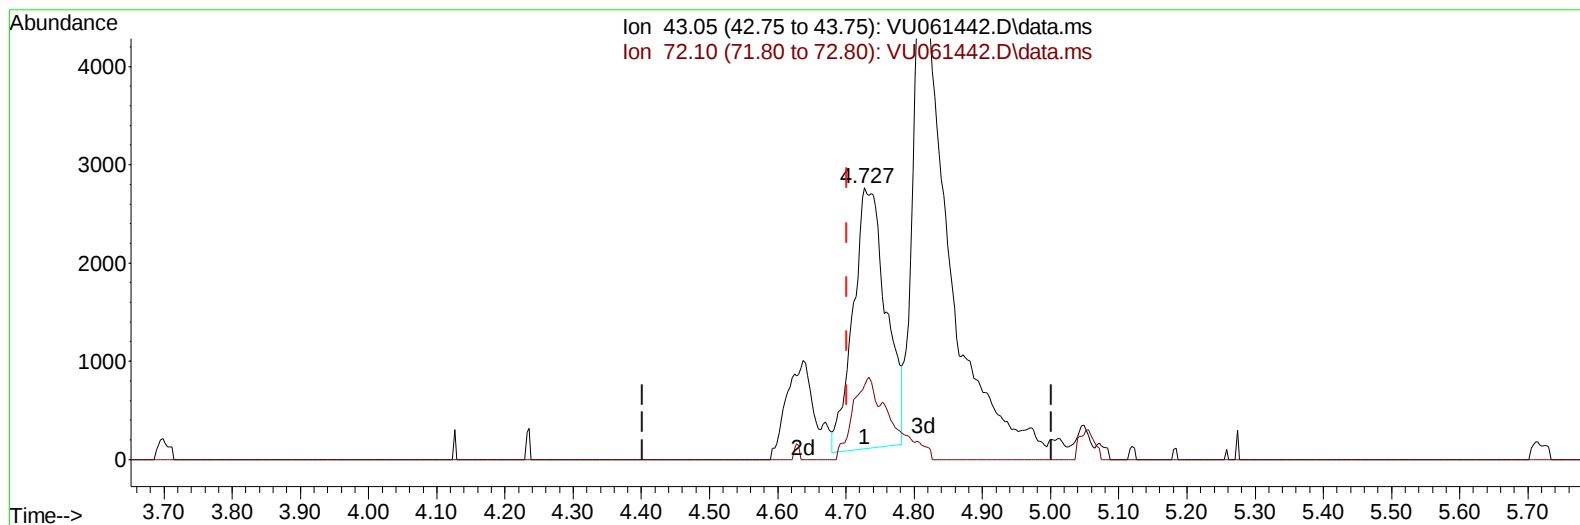

TIC: VU061442.D\data.ms

(21) 2-Butanone (T)

4.727min (+ 0.026) 4.24 ug/L

response 8912

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	31.70	21.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061442.D
Acq On : 05 Nov 2024 06:14
Operator : MD/SY
Sample : P4689-11
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD3

Manual IntegrationsAPPROVED

Quant Time: Nov 05 06:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 05 04:38:45 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
Supervised By :Mahesh Dadoda 11/06/2024

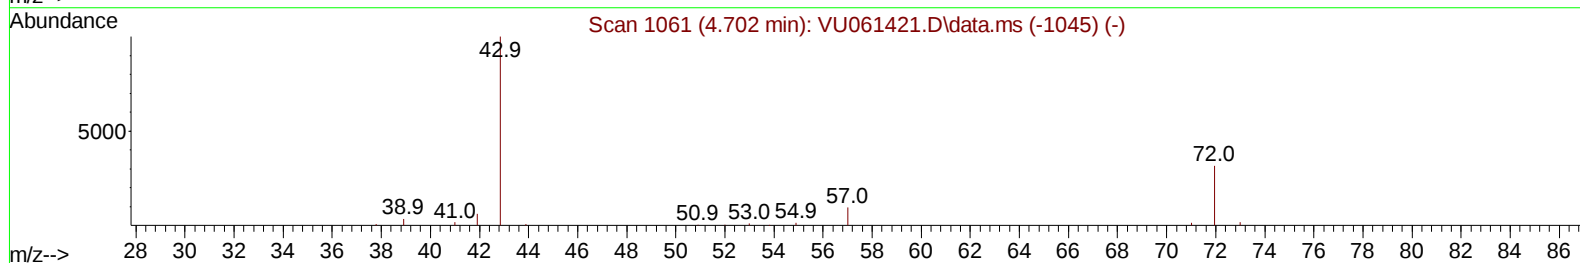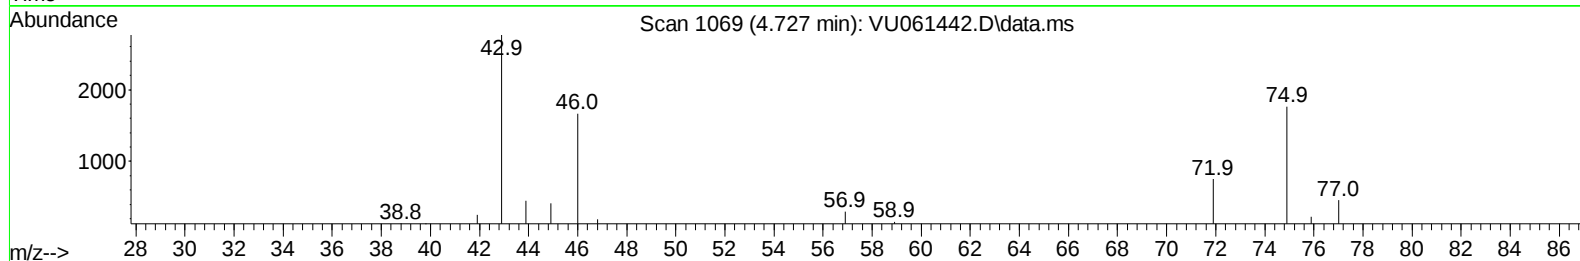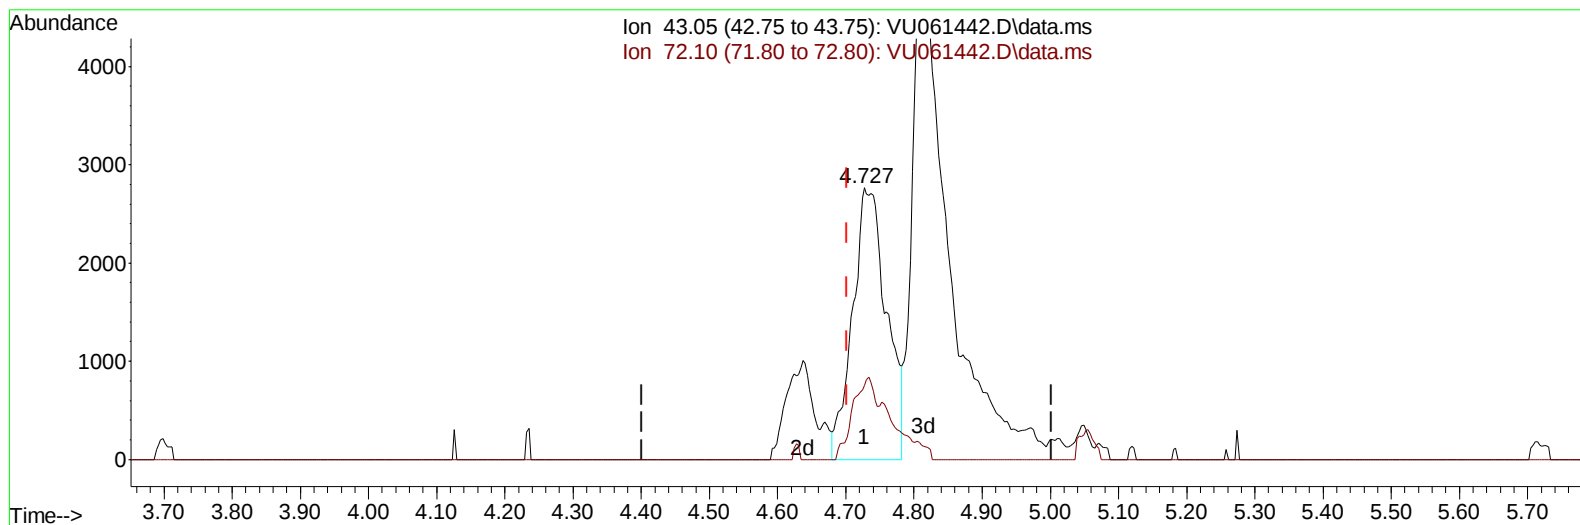

TIC: VU061442.D\data.ms

(21) 2-Butanone (T)

4.727min (+ 0.026) 4.57 ug/L m

response 9603

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	31.70	19.94
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
 Data File : VU061442.D
 Acq On : 05 Nov 2024 06:14
 Operator : MD/SY
 Sample : P4689-11
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CD3

Manual IntegrationsAPPROVED

Quant Time: Nov 05 06:30:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 05 04:38:45 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
 Supervised By :Mahesh Dadoda 11/06/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		151877	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117		143602	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		62123	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		28056	2.719	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	54.400%	
7) Chloroethane-d5	1.911	69		29253	3.093	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	61.800%#	
11) 1,1-Dichloroethene-d2	2.560	65		13778	3.121	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%	
20) 2-Butanone-d5	4.628	46		95754	45.713	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.420%	
24) Chloroform-d	5.052	84		77917	3.979	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.600%	
26) 1,2-Dichloroethane-d4	5.695	65		39605	4.057	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.200%	
32) Benzene-d6	5.718	84		151297	3.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.800%	
36) 1,2-Dichloropropane-d6	6.682	67		48587	3.994	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.800%	
41) Toluene-d8	7.891	98		131865	3.485	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.800%#	
43) trans-1,3-Dichloroprop...	8.177	79		15263	3.074	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.400%	
46) 2-Hexanone-d5	8.627	63		80349	39.506	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.020%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84		38251	4.158	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152		45678	4.152	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.000%	
Target Compounds							Qvalue
13) Acetone	2.647	43		6575	4.956	ug/L	94
21) 2-Butanone	4.727	43		9603m	4.566	ug/L	
47) Tetrachloroethene	8.547	164		10281	1.218	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061442.D
Acq On : 05 Nov 2024 06:14
Operator : MD/SY
Sample : P4689-11
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD3

Manual IntegrationsAPPROVED

Quant Time: Nov 05 06:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 05 04:38:45 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/05/2024
Supervised By :Mahesh Dadoda 11/06/2024

