

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
 Data File : VU061405.D
 Acq On : 04 Nov 2024 14:06
 Operator : MD/SY
 Sample : P4690-05
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF6

Quant Time: Nov 05 00:50:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 01 00:44:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	170954	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	157314	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	69549	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	36809	3.170	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.400%
7) Chloroethane-d5	1.907	69	45416	4.266	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.400%
11) 1,1-Dichloroethene-d2	2.560	65	18715	3.767	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	4.621	46	119557	50.708	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.420%
24) Chloroform-d	5.055	84	101067	4.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.695	65	51852	4.719	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.718	84	201051	4.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
36) 1,2-Dichloropropane-d6	6.682	67	63679	4.778	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.600%
41) Toluene-d8	7.891	98	178410	4.305	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	8.174	79	22051	4.054	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%
46) 2-Hexanone-d5	8.627	63	99851	44.816	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.640%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	48941	4.856	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	59248	4.811	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds					Qvalue	
47) Tetrachloroethene	8.547	164	26060	2.819	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061405.D
Acq On : 04 Nov 2024 14:06
Operator : MD/SY
Sample : P4690-05
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF6


Quant Time: Nov 05 00:50:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 01 00:44:02 2024
Response via : Initial Calibration

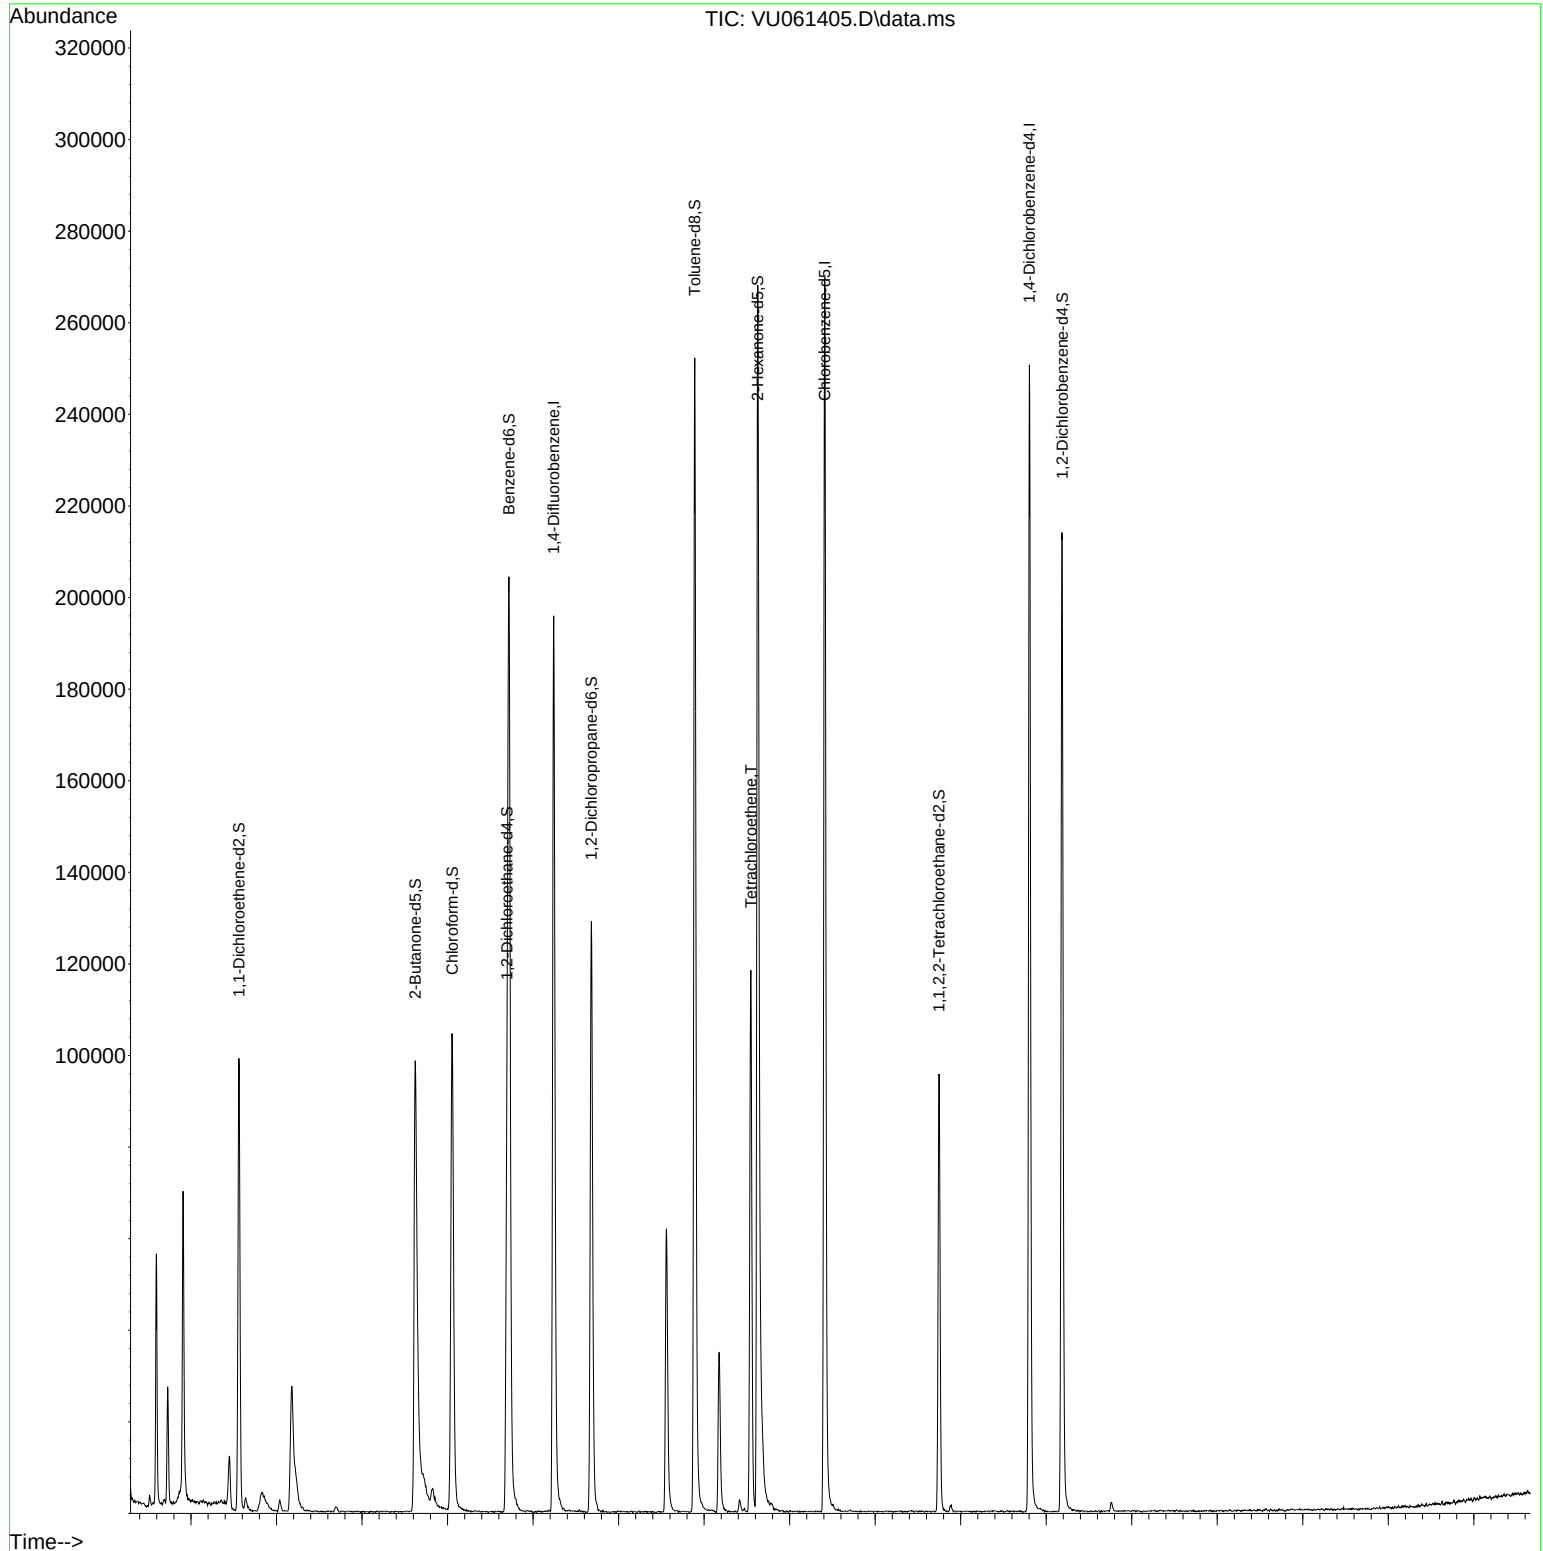

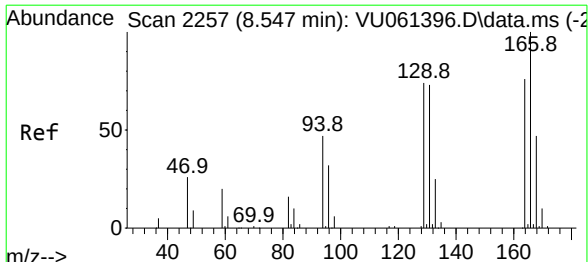

#47
Tetrachloroethene
Concen: 2.819 ug/L
RT: 8.547 min Scan# 22
Delta R.T. -0.000 min
Lab File: VU061405.D
Acq: 04 Nov 2024 14:06

Instrument :
MSVOA_U
ClientSampleId :
C0CF6

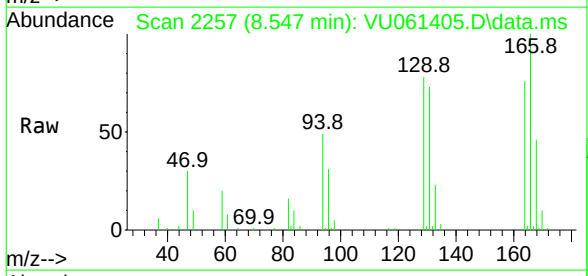

Tgt Ion:	164	Resp:	26060
Ion	Ratio	Lower	Upper
164	100		
129	102.4	69.9	129.7
131	95.5	68.3	126.8
166	130.9	88.8	165.0

