

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
 Data File : VU061406.D
 Acq On : 04 Nov 2024 14:30
 Operator : MD/SY
 Sample : P4690-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rVB	50430	57565	4.69%	0.945%
2	1.727	128	136	148	rVB	39940	49302	4.02%	0.809%
3	1.907	184	192	205	rVB	61048	80492	6.56%	1.321%
4	2.560	384	395	410	rBV	89273	146187	11.91%	2.399%
5	2.824	454	477	512	rBV2	13202	63458	5.17%	1.041%
6	3.177	570	587	609	rBV	79990	183529	14.95%	3.011%
7	4.621	1018	1036	1060	rBV2	147359	415755	33.87%	6.822%
8	5.052	1155	1170	1192	rBV2	94895	212462	17.31%	3.486%
9	5.718	1355	1377	1409	rBV2	190338	500689	40.80%	8.216%
10	6.242	1527	1540	1561	rBV	209591	408573	33.29%	6.704%
11	6.682	1662	1677	1703	rBV	118626	236119	19.24%	3.874%
12	7.560	1936	1950	1977	rBV	56919	106171	8.65%	1.742%
13	7.891	2039	2053	2072	rBV	231773	412439	33.60%	6.768%
14	8.174	2128	2141	2160	rBV	32573	59611	4.86%	0.978%
15	8.544	2243	2256	2273	rBV	716373	1227323	100.00%	20.139%
16	8.627	2273	2282	2316	rVB2	245350	501782	40.88%	8.234%
17	9.409	2513	2525	2548	rBV	284686	507142	41.32%	8.321%
18	10.749	2929	2942	2962	rBV2	87597	146043	11.90%	2.396%
19	11.804	3258	3270	3295	rBV	260525	439541	35.81%	7.212%
20	12.187	3377	3389	3413	rBV	198822	340196	27.72%	5.582%

Sum of corrected areas: 6094379




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061406.D
Acq On : 04 Nov 2024 14:30
Operator : MD/SY
Sample : P4690-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

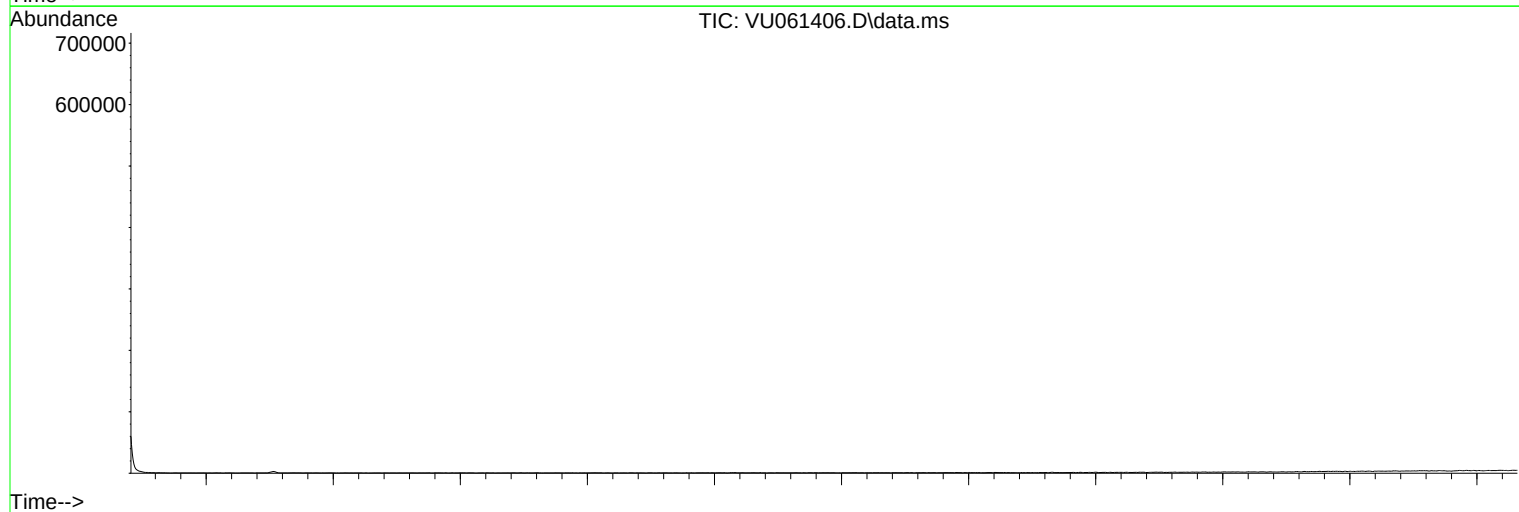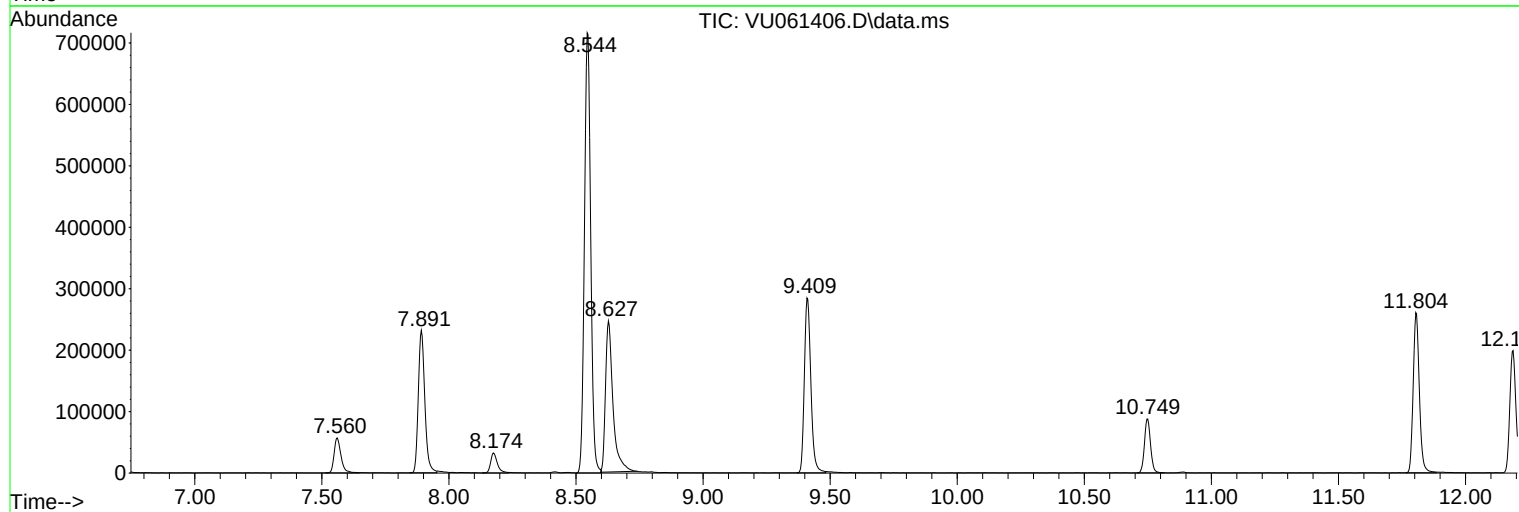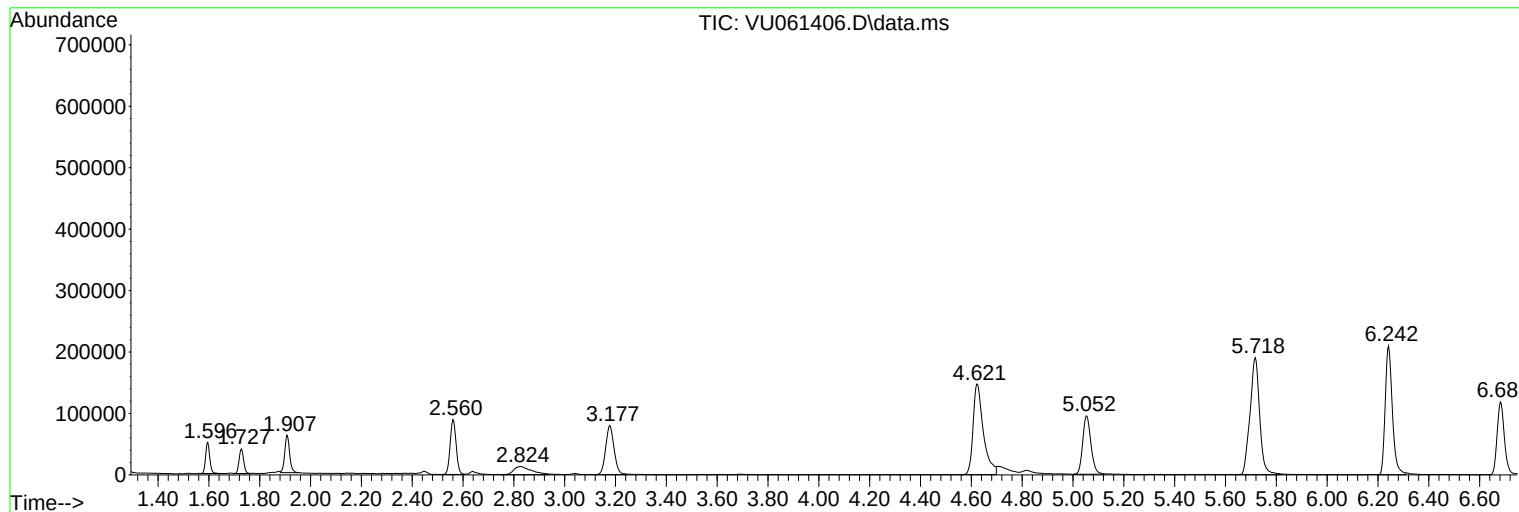

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061406.D
Acq On : 04 Nov 2024 14:30
Operator : MD/SY
Sample : P4690-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061406.D
Acq On : 04 Nov 2024 14:30
Operator : MD/SY
Sample : P4690-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------