
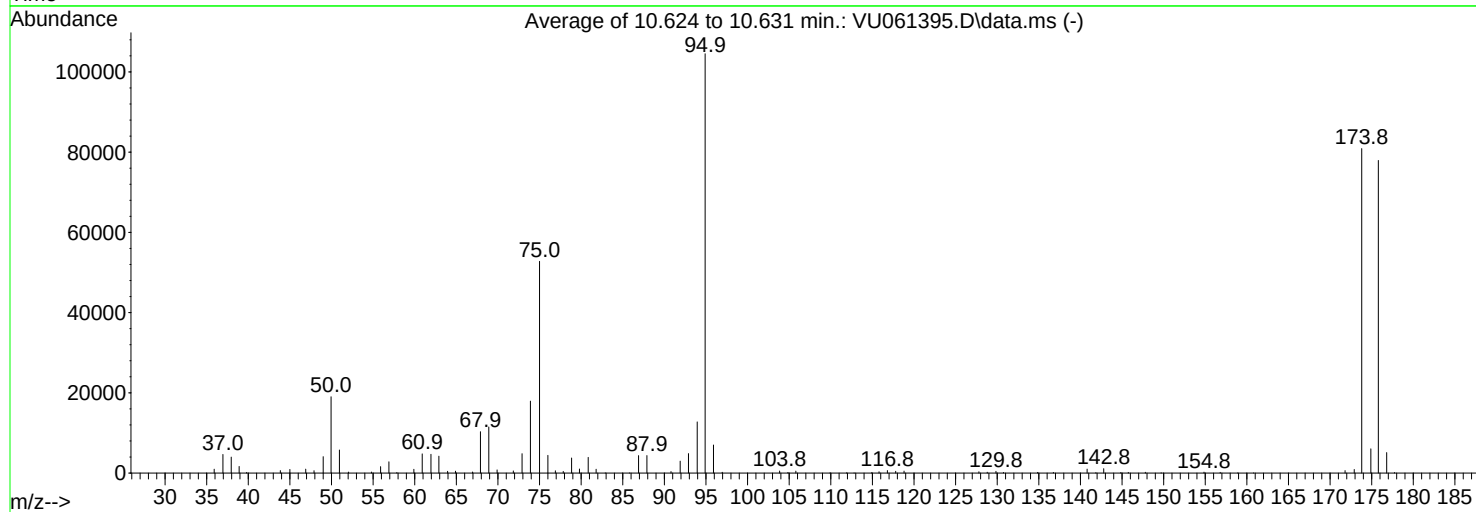


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110424\
Data File : VU061395.D
Acq On : 04 Nov 2024 09:16
Operator : MD/SY
Sample : BFB019
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB019

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 06 00:52:59 2024

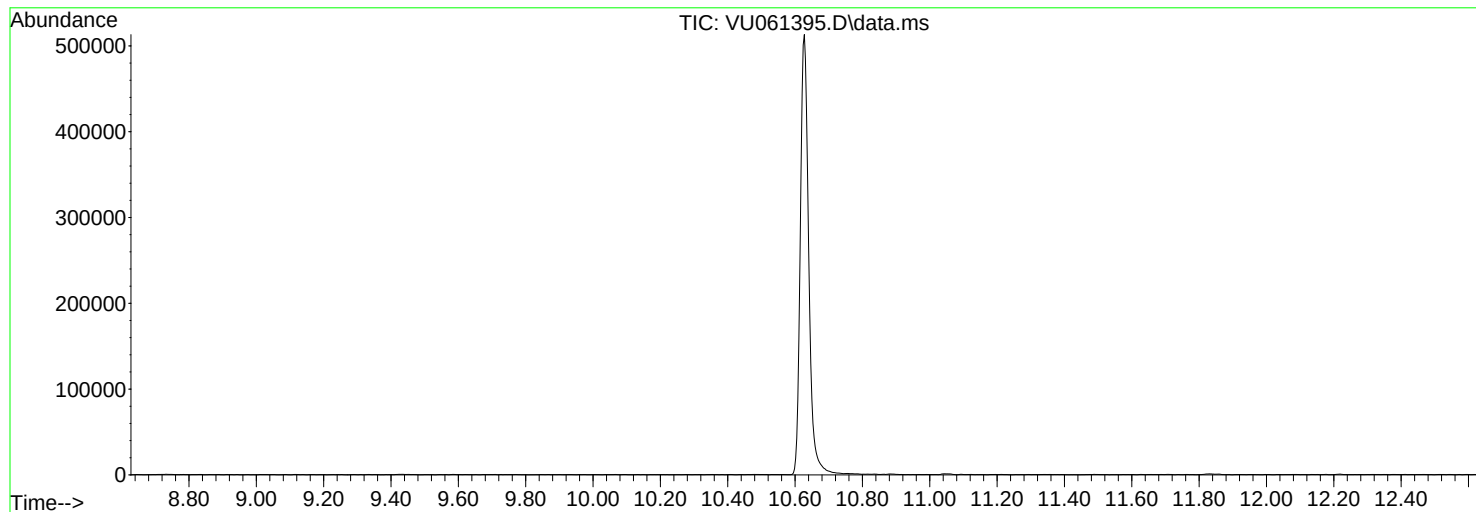

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	19024	PASS
75	95	30	80	50.5	52784	PASS
95	95	100	100	100.0	104536	PASS
96	95	5	9	6.7	7006	PASS
173	174	0.00	2	1.1	895	PASS
174	95	50	120	77.4	80893	PASS
175	174	5	9	7.5	6049	PASS
176	174	95	101	96.3	77936	PASS
177	176	5	9	6.5	5104	PASS

m/z	Abundance
43.80	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	1095.0
36.90	4878.0
37.90	3992.0
38.90	1703.0
39.80	158.0
43.90	953.0
45.00	902.0
46.90	913.0
47.90	606.0
49.00	4250.0
49.90	19064.0
51.00	5969.0
52.00	266.0
54.80	298.0
55.90	1728.0
56.90	2878.0
57.90	134.0
59.90	955.0
60.90	4667.0
61.90	4857.0
62.90	4352.0
63.90	508.0
64.90	540.0
66.90	294.0
67.90	10463.0
68.90	11409.0
69.90	817.0
71.90	573.0
72.90	4874.0
73.90	18352.0
75.00	53272.0
76.00	4496.0
76.90	611.0
77.90	452.0
78.80	3892.0
79.80	1061.0
80.90	3816.0
81.80	991.0
85.80	106.0
86.90	4344.0
87.90	4514.0
90.80	384.0
91.90	3030.0
92.90	4917.0
94.00	12904.0
94.90	104664.0
95.90	7092.0
97.00	188.0
103.90	576.0
104.80	167.0
105.80	523.0
111.90	110.0
114.90	132.0
115.80	341.0
116.80	592.0
117.80	382.0
118.80	498.0
127.80	312.0
128.80	212.0
129.80	499.0
130.80	138.0
134.80	182.0
136.80	175.0
140.80	1003.0
141.80	103.0
142.80	1094.0
144.90	169.0
145.80	189.0
147.80	226.0
149.70	108.0
154.80	275.0
156.80	202.0
158.90	112.0
160.80	112.0
171.80	579.0
172.90	821.0
173.80	80136.0
174.90	6009.0
175.80	76440.0
176.80	5182.0
177.80	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	1028.0
36.90	4780.0
38.00	4162.0
38.90	1685.0
39.80	166.0
43.90	936.0
45.00	955.0
46.90	1032.0
47.90	636.0
49.00	4213.0
50.00	19448.0
51.00	5855.0
52.00	254.0
54.80	269.0
55.90	1605.0
56.90	2859.0
57.90	156.0
59.90	957.0
60.90	4951.0
61.90	4765.0
62.90	4348.0
64.00	443.0
64.90	498.0
67.00	286.0
67.90	10629.0
68.90	11885.0
69.90	819.0
71.90	546.0
72.90	4965.0
73.90	18352.0
75.00	54080.0
76.00	4514.0
76.90	601.0
77.90	405.0
78.90	3855.0
79.80	1057.0
80.80	4065.0
81.80	982.0
86.90	4505.0
87.90	4502.0
90.80	400.0
91.90	3054.0
92.90	5018.0
94.00	13121.0
94.90	107408.0
95.90	7250.0
97.00	200.0
103.90	530.0
104.80	183.0
105.80	496.0
109.90	100.0
111.90	107.0
114.90	119.0
115.80	339.0
116.80	642.0
117.80	459.0
118.80	511.0
127.80	361.0
128.80	226.0
129.80	457.0
130.80	157.0
134.90	168.0
136.70	163.0
140.80	1021.0
141.80	113.0
142.80	1109.0
144.90	144.0
145.70	181.0
147.80	191.0
149.70	104.0
154.80	247.0
156.80	178.0
171.80	636.0
172.90	927.0
173.80	83088.0
174.90	6179.0
175.80	80144.0
176.80	5223.0
177.80	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	787.0
37.00	4288.0
38.00	3817.0
38.90	1577.0
39.80	145.0
43.90	882.0
45.00	864.0
46.90	1009.0
47.90	568.0
49.00	3816.0
50.00	18560.0
50.90	5441.0
52.10	224.0
54.80	219.0
55.90	1489.0
56.90	2713.0
57.80	128.0
59.90	910.0
60.90	4760.0
62.00	4420.0
62.90	3952.0
64.00	403.0
64.90	414.0
67.00	259.0
67.90	9856.0
68.90	11182.0
69.90	758.0
71.80	499.0
72.90	4690.0
73.90	17096.0
75.00	51000.0
76.00	4259.0
76.90	538.0
77.80	392.0
78.90	3525.0
79.80	946.0
80.80	3860.0
81.80	883.0
82.90	102.0
86.90	4216.0
87.90	4104.0
90.80	382.0
91.90	2850.0
92.90	4640.0
93.90	12237.0
94.90	101536.0
95.90	6676.0
96.90	216.0
103.80	457.0
104.90	170.0
105.80	467.0
112.80	113.0
115.80	324.0
116.80	670.0
117.80	484.0
118.80	514.0
127.80	334.0
128.80	220.0
129.90	375.0
130.70	167.0
134.90	170.0
136.70	163.0
140.80	974.0
141.90	107.0
142.80	1103.0
144.80	133.0
145.70	134.0
147.80	198.0
154.90	209.0
156.80	151.0
171.80	645.0
172.90	936.0
173.80	79456.0
174.90	5960.0
175.80	77224.0
176.80	4906.0
177.70	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019