

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110524\
 Data File : VU061479.D
 Acq On : 06 Nov 2024 03:04
 Operator : MD/SY
 Sample : P4714-16
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 06 03:42:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 06 00:52:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	142632	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	136498	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	58748	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	46717	4.822	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.400%
7) Chloroethane-d5	1.911	69	43162	4.859	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.560	65	21274	5.132	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.600%
20) 2-Butanone-d5	4.628	46	101286	51.488	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.980%
24) Chloroform-d	5.052	84	95219	5.177	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
26) 1,2-Dichloroethane-d4	5.695	65	48153	5.253	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.718	84	198474	5.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
36) 1,2-Dichloropropane-d6	6.682	67	61239	5.296	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.000%
41) Toluene-d8	7.891	98	178054	4.951	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	8.174	79	18326	3.883	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%
46) 2-Hexanone-d5	8.627	63	91506	47.333	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.660%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	46092	5.271	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	57647	5.541	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%
Target Compounds						
					Qvalue	
35) Methylcyclohexane	6.682	83	14201	0.777	ug/L #	21
37) 1,2-Dichloropropane	6.679	63	6549	0.612	ug/L #	89
49) Dibromochloromethane	8.547	129	2322	0.266	ug/L #	12
61) 1,2,3-Trichloropropane	11.804	75	7267	1.242	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110524\
Data File : VU061479.D
Acq On : 06 Nov 2024 03:04
Operator : MD/SY
Sample : P4714-16
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Nov 06 03:42:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 00:52:59 2024
Response via : Initial Calibration




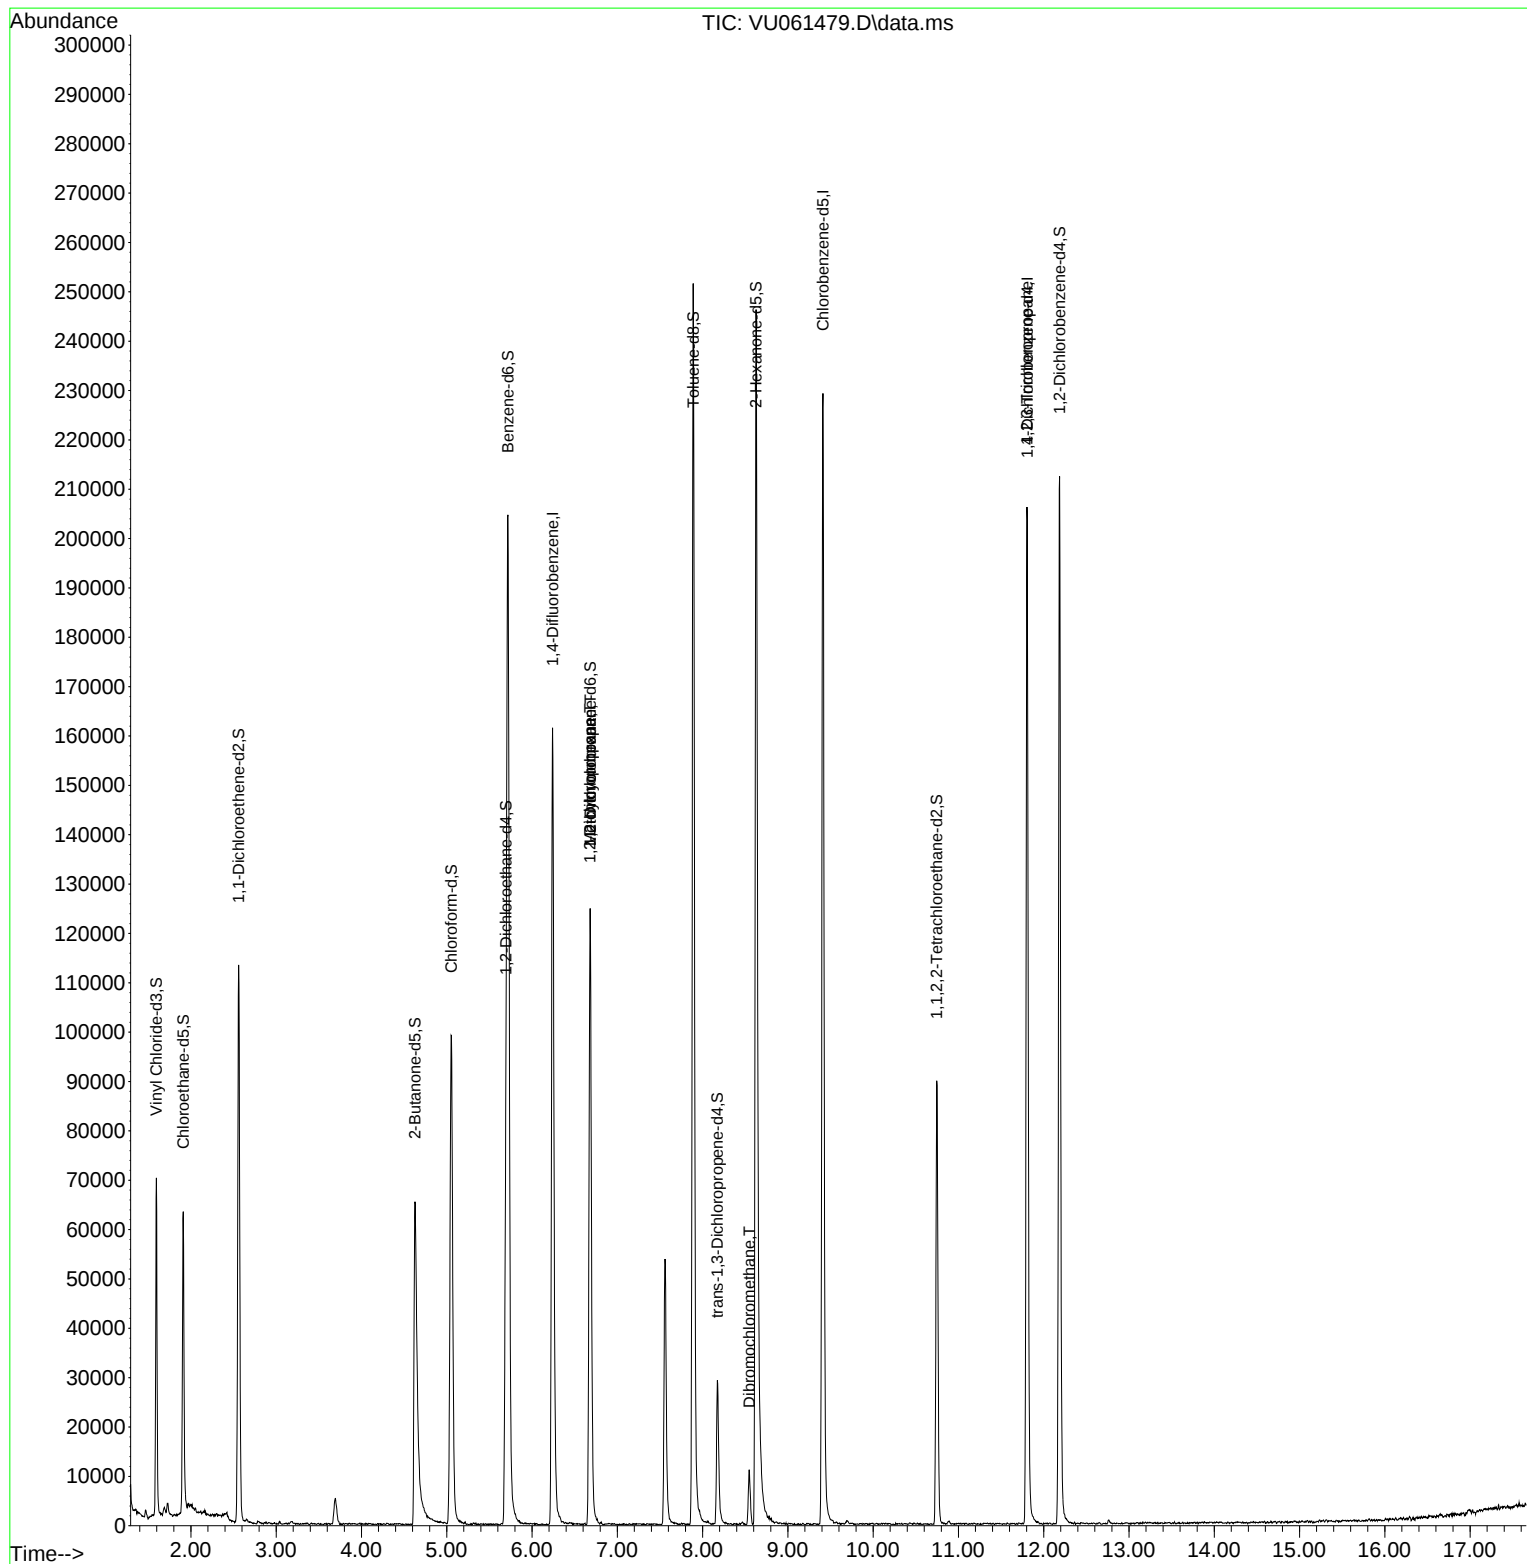


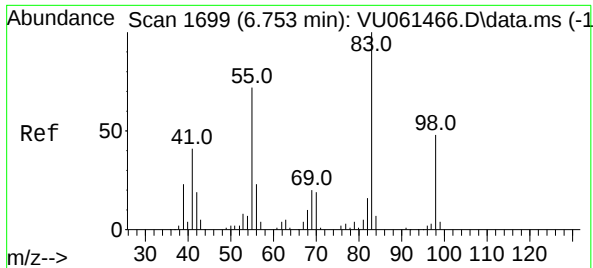

#35
Methylcyclohexane
Concen: 0.777 ug/L
RT: 6.682 min Scan# 1677
Delta R.T. -0.071 min
Lab File: VU061479.D
Acq: 06 Nov 2024 03:04




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 83 Resp: 14201
Ion Ratio Lower Upper
83 100
55 0.0 55.9 83.9#
98 0.1 35.9 53.9#

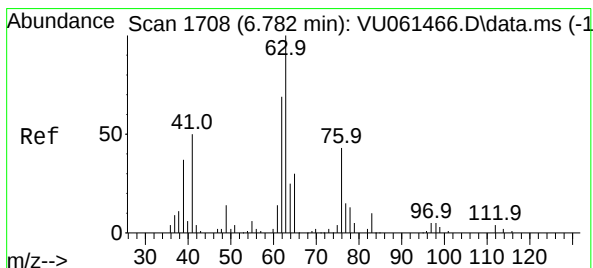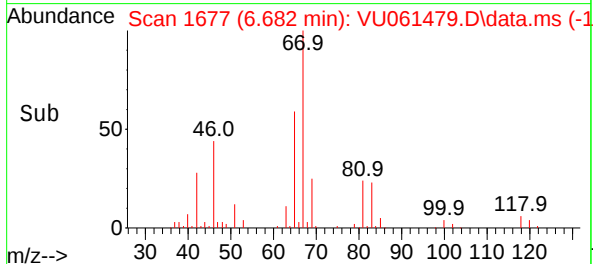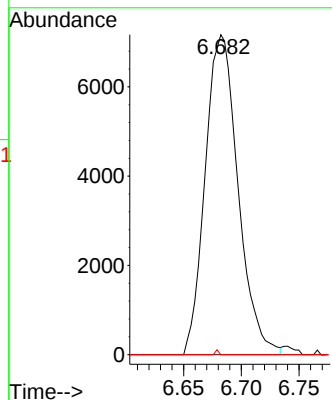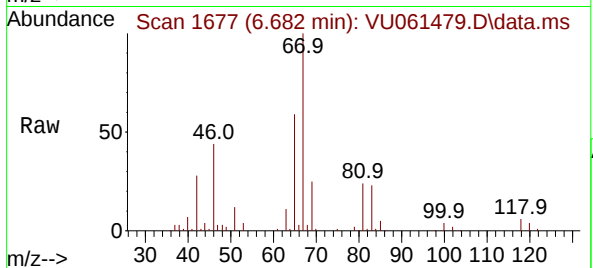

#37
1,2-Dichloropropane
Concen: 0.612 ug/L
RT: 6.679 min Scan# 1676
Delta R.T. -0.103 min
Lab File: VU061479.D
Acq: 06 Nov 2024 03:04

Tgt Ion: 63 Resp: 6549
Ion Ratio Lower Upper
63 100
112 0.0 3.0 4.4#

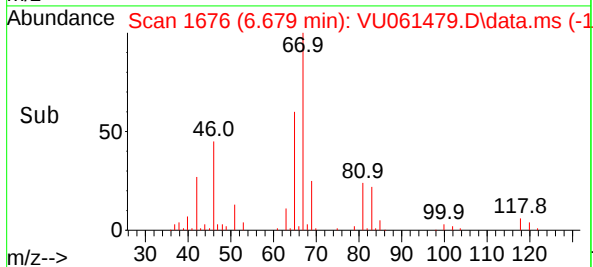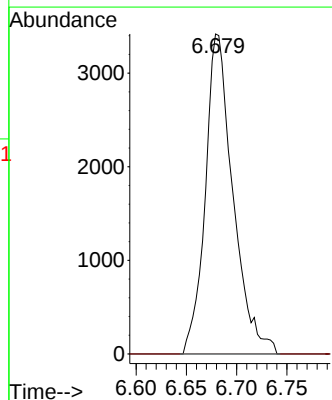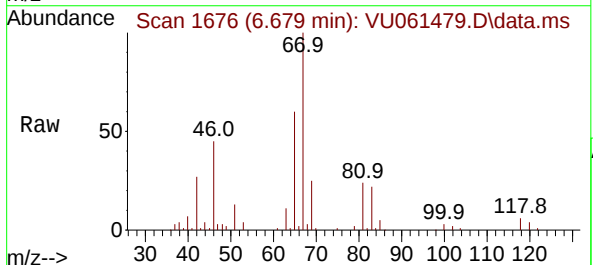

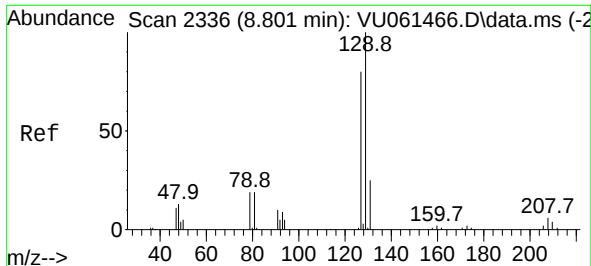

#49

Dibromochloromethane

Concen: 0.266 ug/L

RT: 8.547 min Scan# 21

Delta R.T. -0.254 min MSVOA_U

Lab File: VU061479.D

Acq: 06 Nov 2024 03:04

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:129 Resp: 2322

Ion Ratio Lower Upper

129 100

127 0.0 51.8 96.2#

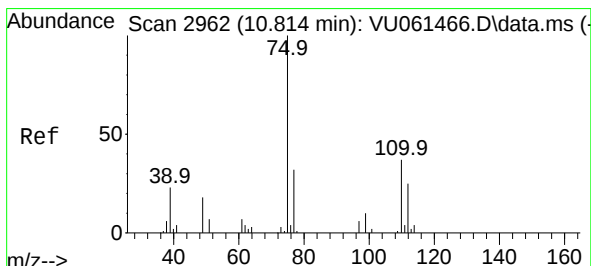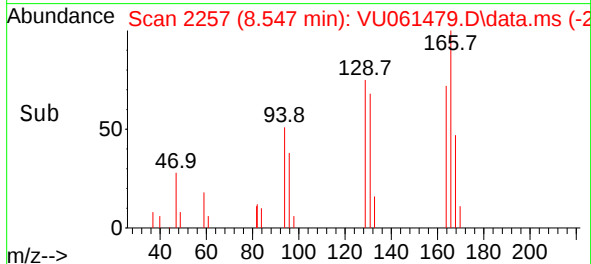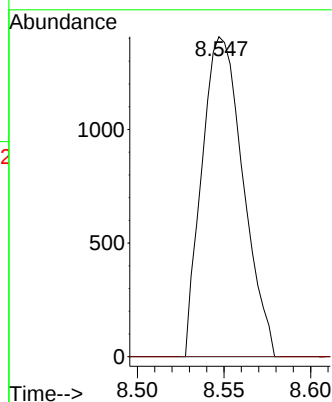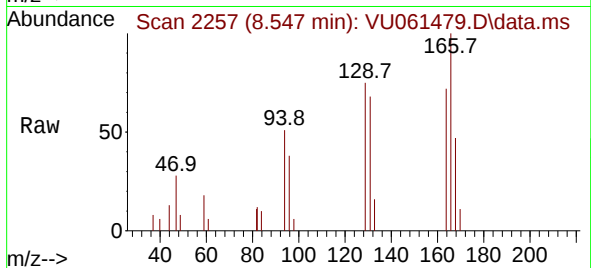

#61

1,2,3-Trichloropropane

Concen: 1.242 ug/L

RT: 11.804 min Scan# 3270

Delta R.T. 0.990 min

Lab File: VU061479.D

Acq: 06 Nov 2024 03:04

Tgt Ion: 75 Resp: 7267

Ion Ratio Lower Upper

75 100

110 2.0 28.8 43.2#

77 33.4 25.7 38.5

