

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110524\
 Data File : VU061470.D
 Acq On : 05 Nov 2024 23:24
 Operator : MD/SY
 Sample : P4689-17
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CE8

Quant Time: Nov 06 00:54:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 06 00:52:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	148737	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	141005	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	59966	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	49137	4.863	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.200%
7) Chloroethane-d5	1.911	69	49580	5.353	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.000%
11) 1,1-Dichloroethene-d2	2.560	65	22388	5.179	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.600%
20) 2-Butanone-d5	4.624	46	111164	54.190	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.380%
24) Chloroform-d	5.052	84	98827	5.153	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.692	65	52090	5.449	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.000%
32) Benzene-d6	5.718	84	209267	5.267	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
36) 1,2-Dichloropropane-d6	6.682	67	62998	5.274	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.400%
41) Toluene-d8	7.891	98	184061	4.955	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	8.174	79	19847	4.070	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.627	63	95177	47.659	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.320%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	46413	5.138	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	58439	5.503	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.000%
Target Compounds						
13) Acetone	2.641	43	5591	4.303	ug/L	96
21) 2-Butanone	4.721	43	9232	4.482	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110524\
Data File : VU061470.D
Acq On : 05 Nov 2024 23:24
Operator : MD/SY
Sample : P4689-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CE8

Quant Time: Nov 06 00:54:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 00:52:59 2024
Response via : Initial Calibration

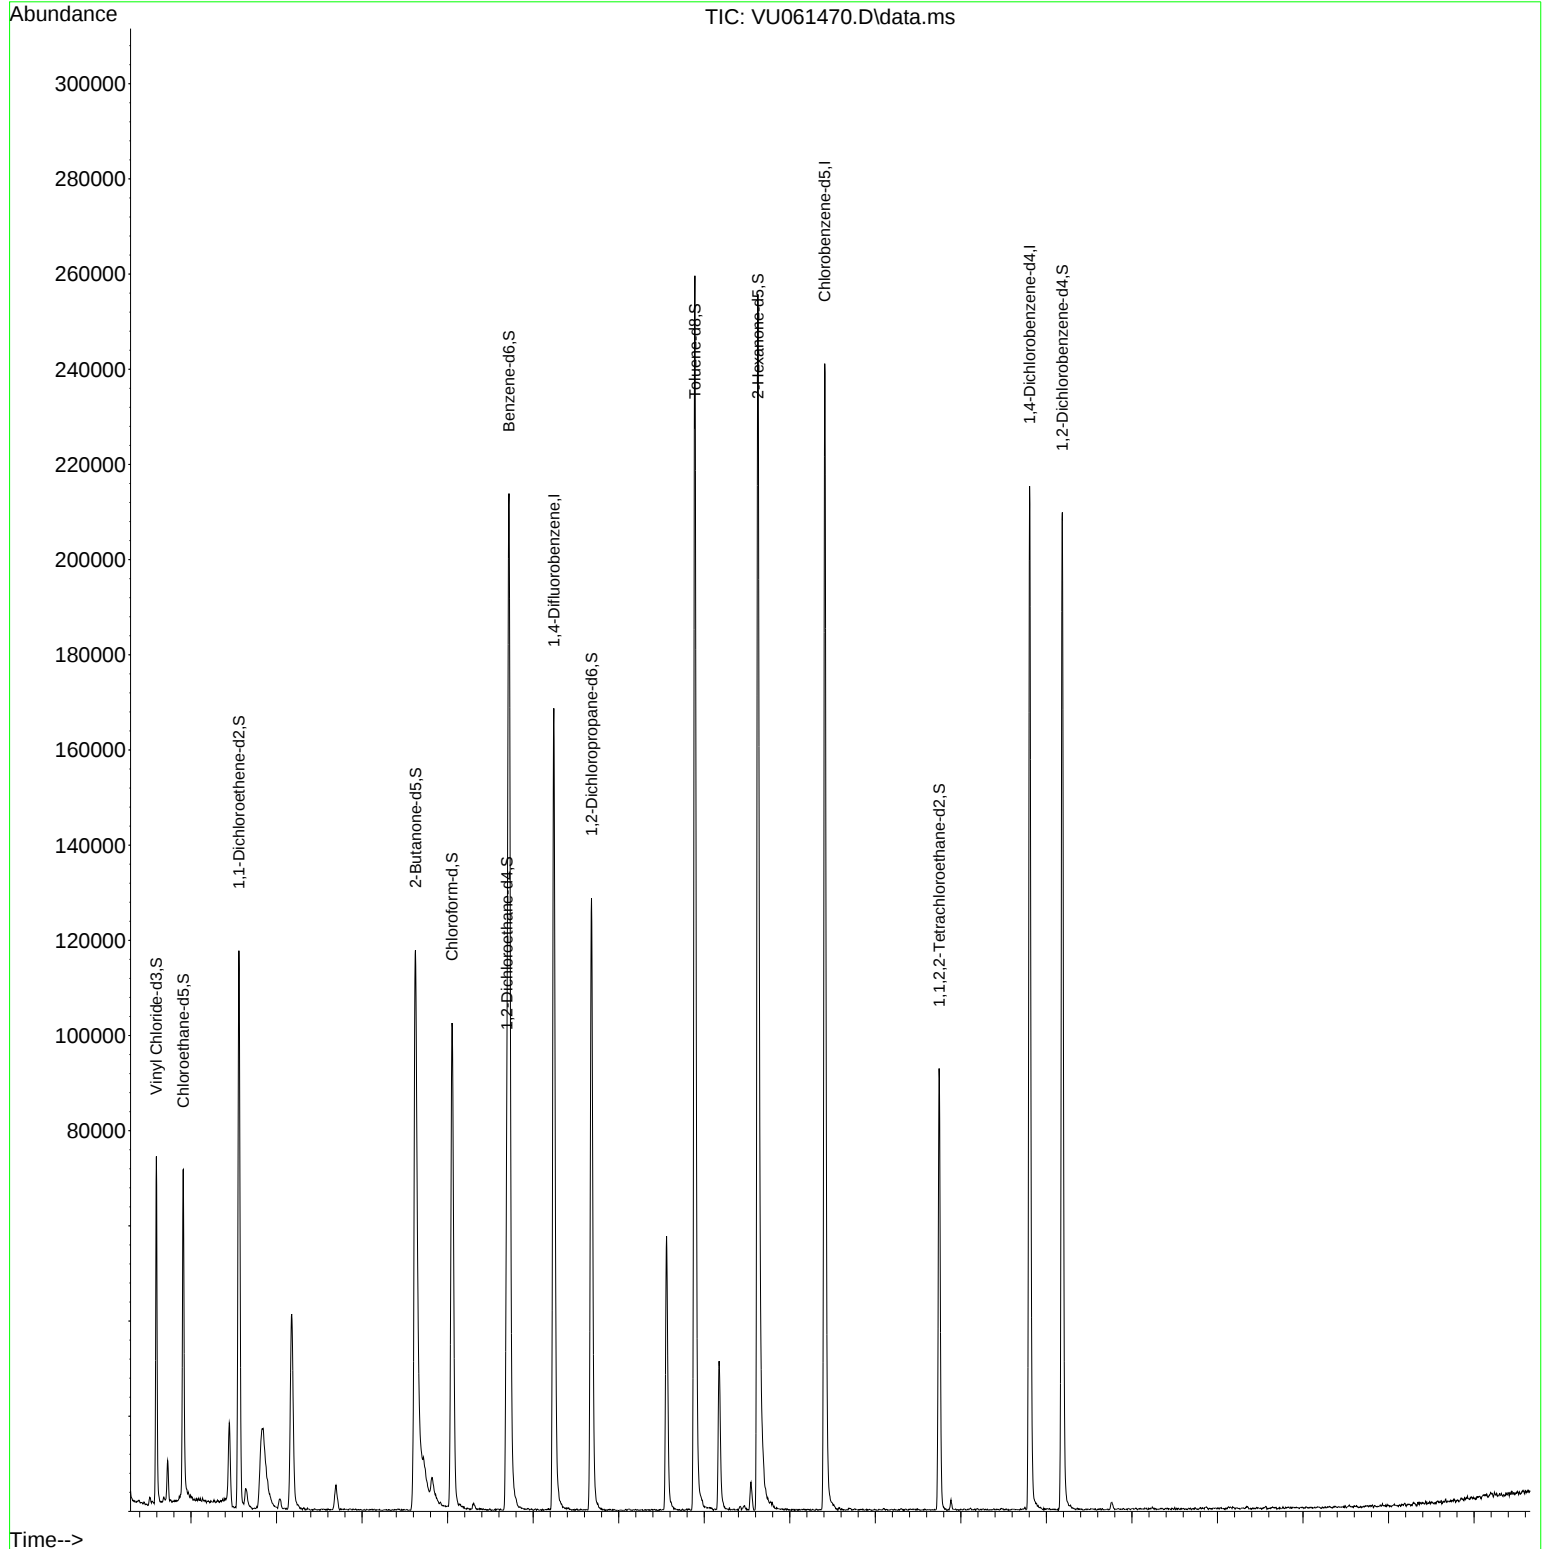

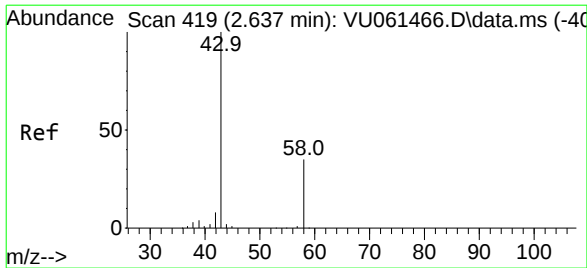

#13

Acetone

Concen: 4.303 ug/L

RT: 2.641 min Scan# 42

Delta R.T. 0.003 min

Lab File: VU061470.D

Acq: 05 Nov 2024 23:24

Instrument :

MSVOA_U

ClientSampleId :





C0CE8

Tgt Ion: 43 Resp: 5591

Ion Ratio Lower Upper

43 100

58 34.0 0.0 73.2

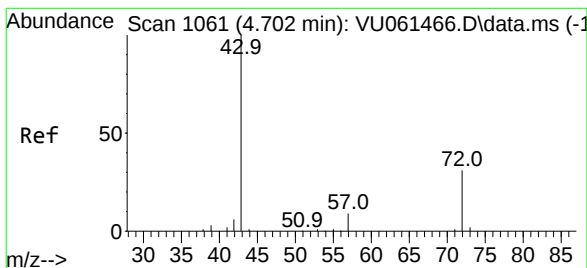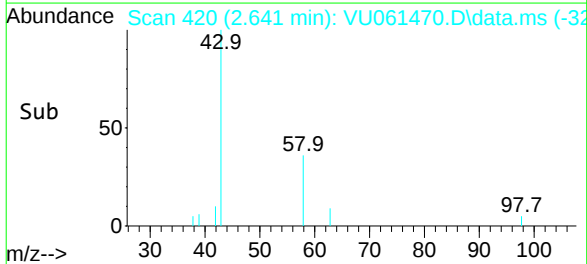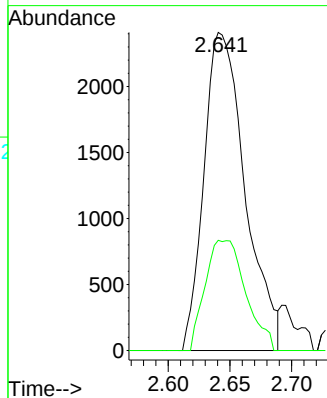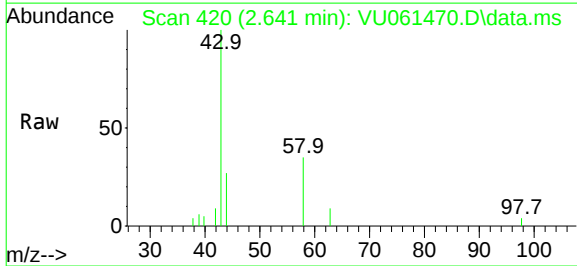

#21

2-Butanone

Concen: 4.482 ug/L

RT: 4.721 min Scan# 1067

Delta R.T. 0.019 min

Lab File: VU061470.D

Acq: 05 Nov 2024 23:24

Tgt Ion: 43 Resp: 9232

Ion Ratio Lower Upper

43 100

72 11.7 15.9 47.6#

